



MULTIPHOTON MICROSCOPY

*Methods for Cell Analysis Course
BioVis – Uppsala, 2014*

**Matyas Molnar
Dirk Pacholsky**



UPPSALA
UNIVERSITET

SciLifeLab BioVis platform

Information

Information given here about 2 Photon microscopy were mainly taken from these sources:

Background information on 2-Photon microscopy:

<http://micro.magnet.fsu.edu/primer/techniques/fluorescence/multiphoton/multiphotonintro.html>

The microscopes:


Zeiss LSM 710 NLO; <http://www.zeiss.com>

Olympus Fluoview 1000 MPE, <http://www.olympusamerica.com>


Spectra-Physics Laser:

<http://www.newport.com/store/selectcountry.aspx?newpurl=/Lasers/361887/1033/catalog.aspx>

Schematic drawing of LSM


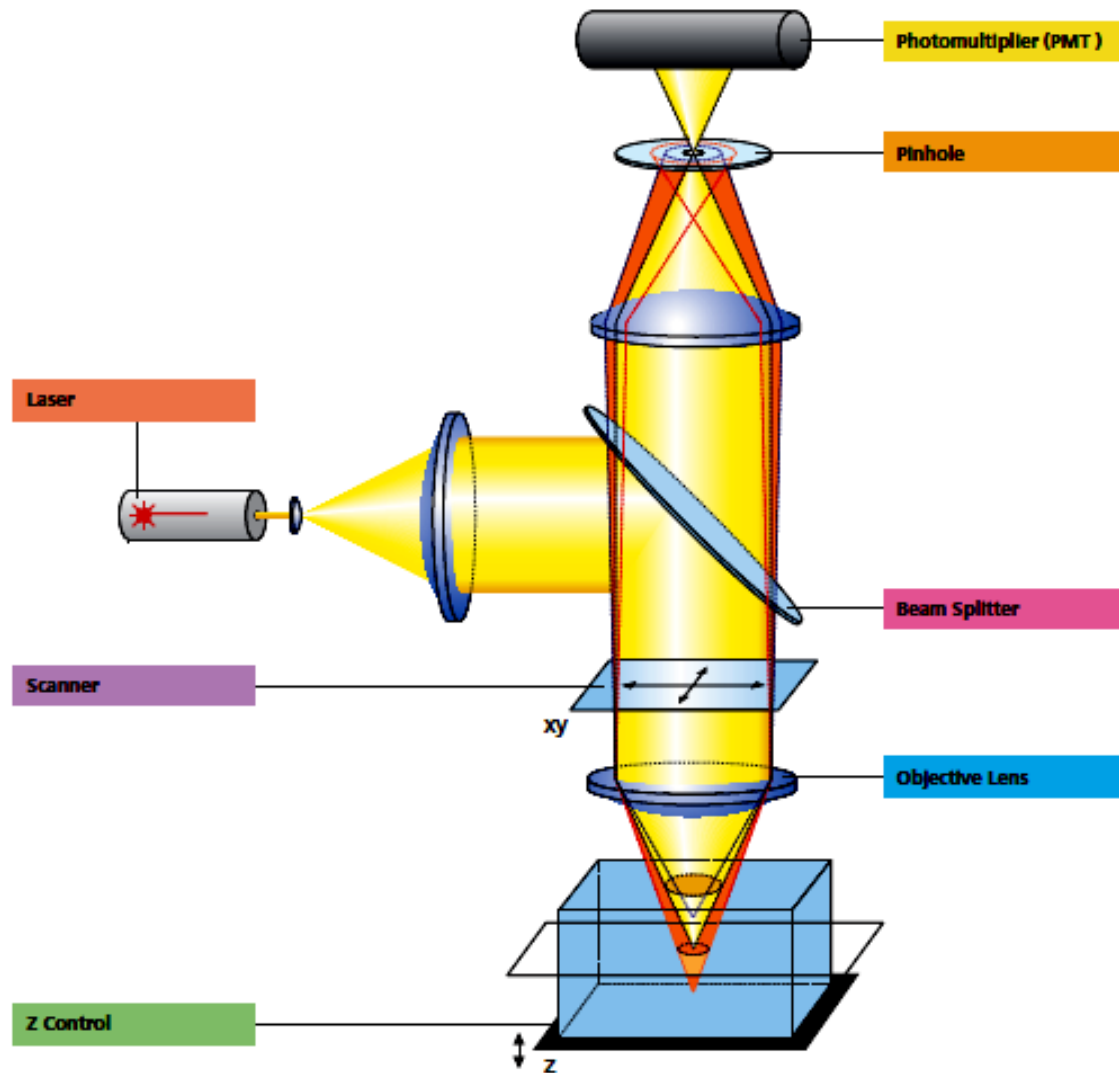


Why use 2-Photon microscopy?

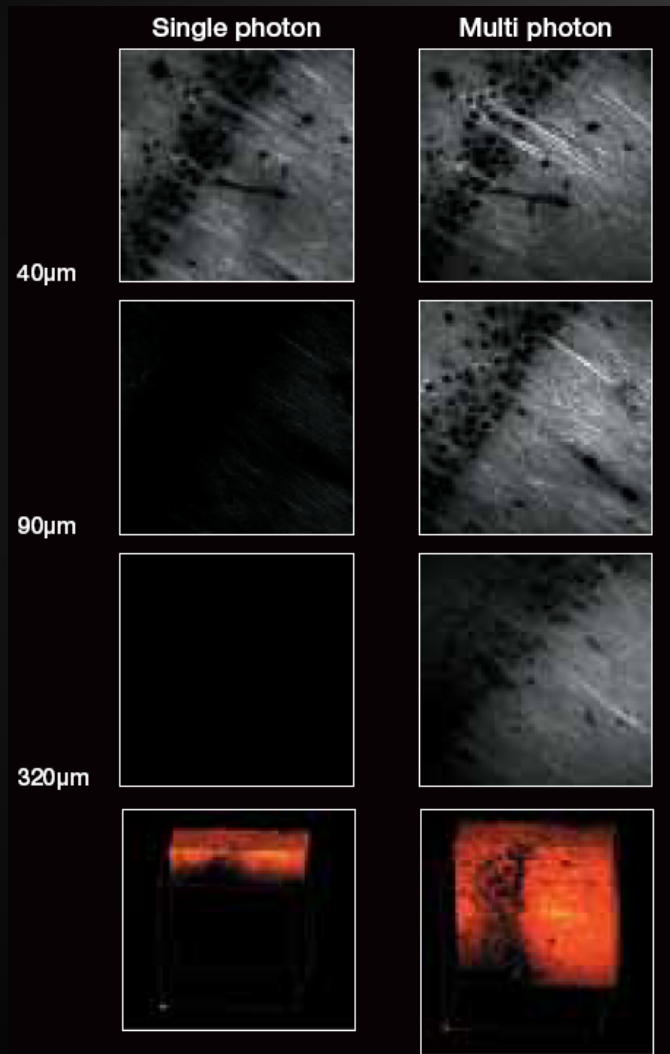

Multiphoton

LSM/ widefield

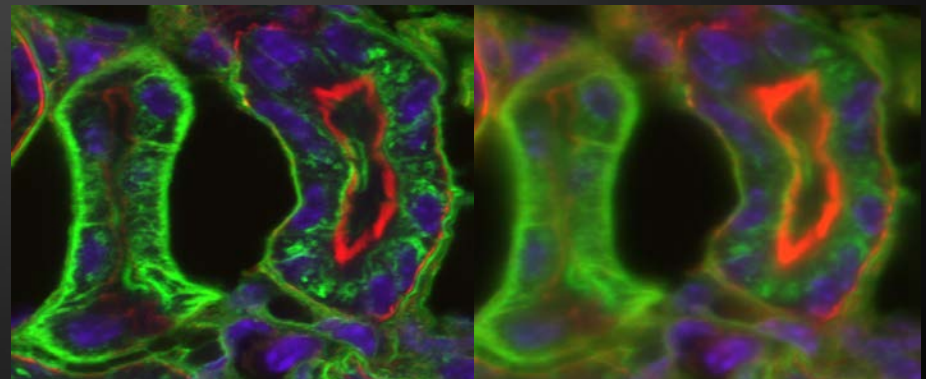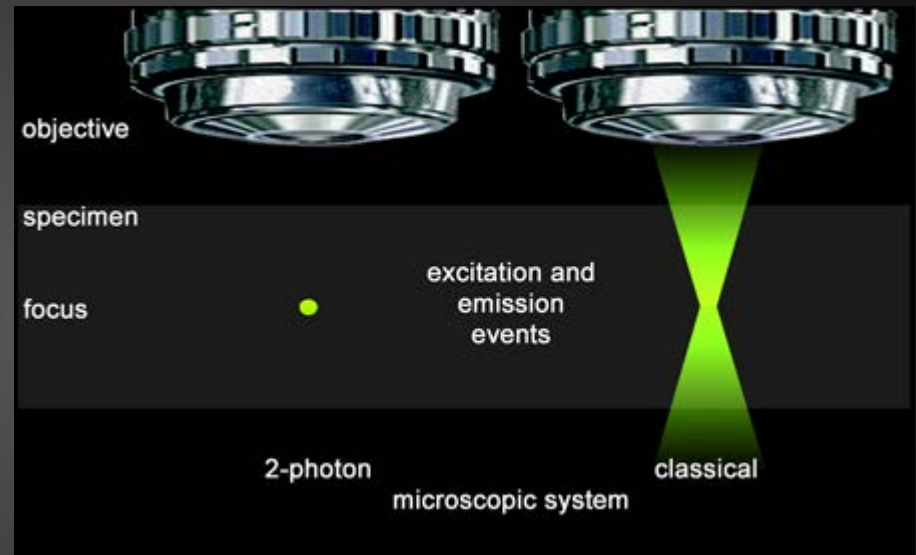

The message to keep in mind


A multiphoton microscope gives you the opportunity to get images from **deep** (e.g. 500 nm) within (**living**) tissue, whilst **photodamaging only the imaged volume**.

A Multiphoton microscope is a point scanning system which **excites fluorophores within the Focus volume only**.

Therefore you collect emission light from this volume only, enabling you to acquire optical slices, **without the use of confocal pinholes**.

Beside this, one is able to photomanipulate tissue/cells within a very small volume.


THE THEORY OF 2PM

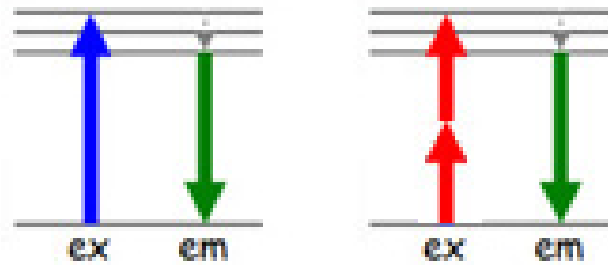


1P

2P

z

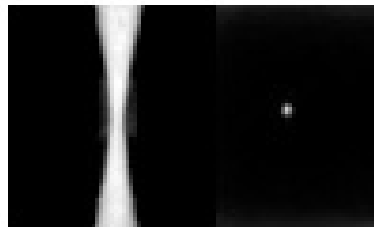

Theory for 2PM : The 1Photon Excitation

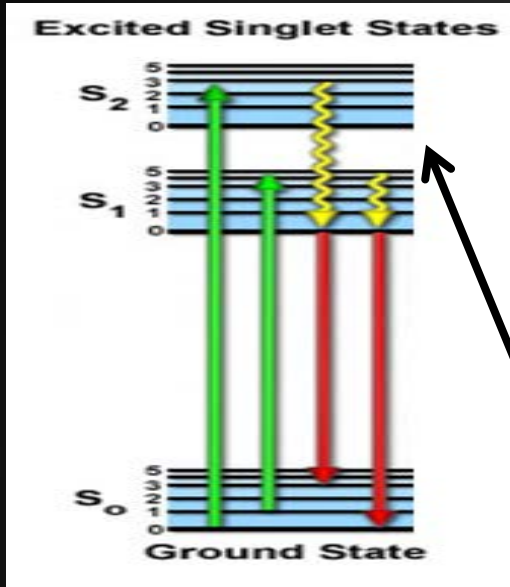

Stokes shift


- Illuminate a fluorophore with appropriate λ of light
- 1 (excitation) photon absorbed gives 1 emission photon

← BUT


- emission photon will have less energy i.e. longer λ than excitation photon

AND

- it's λ and energy vary due to which S_0 level (0,1,2,3) the fluorophore relaxes
- Fluorescence - photons with different λ emission curve is bell shaped

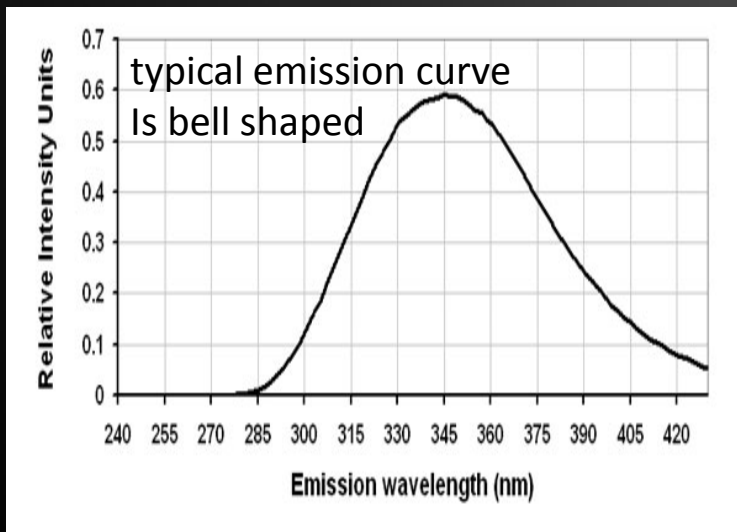

Theory for 2PM : $\lambda \sim E$ - The Energy of a Photon

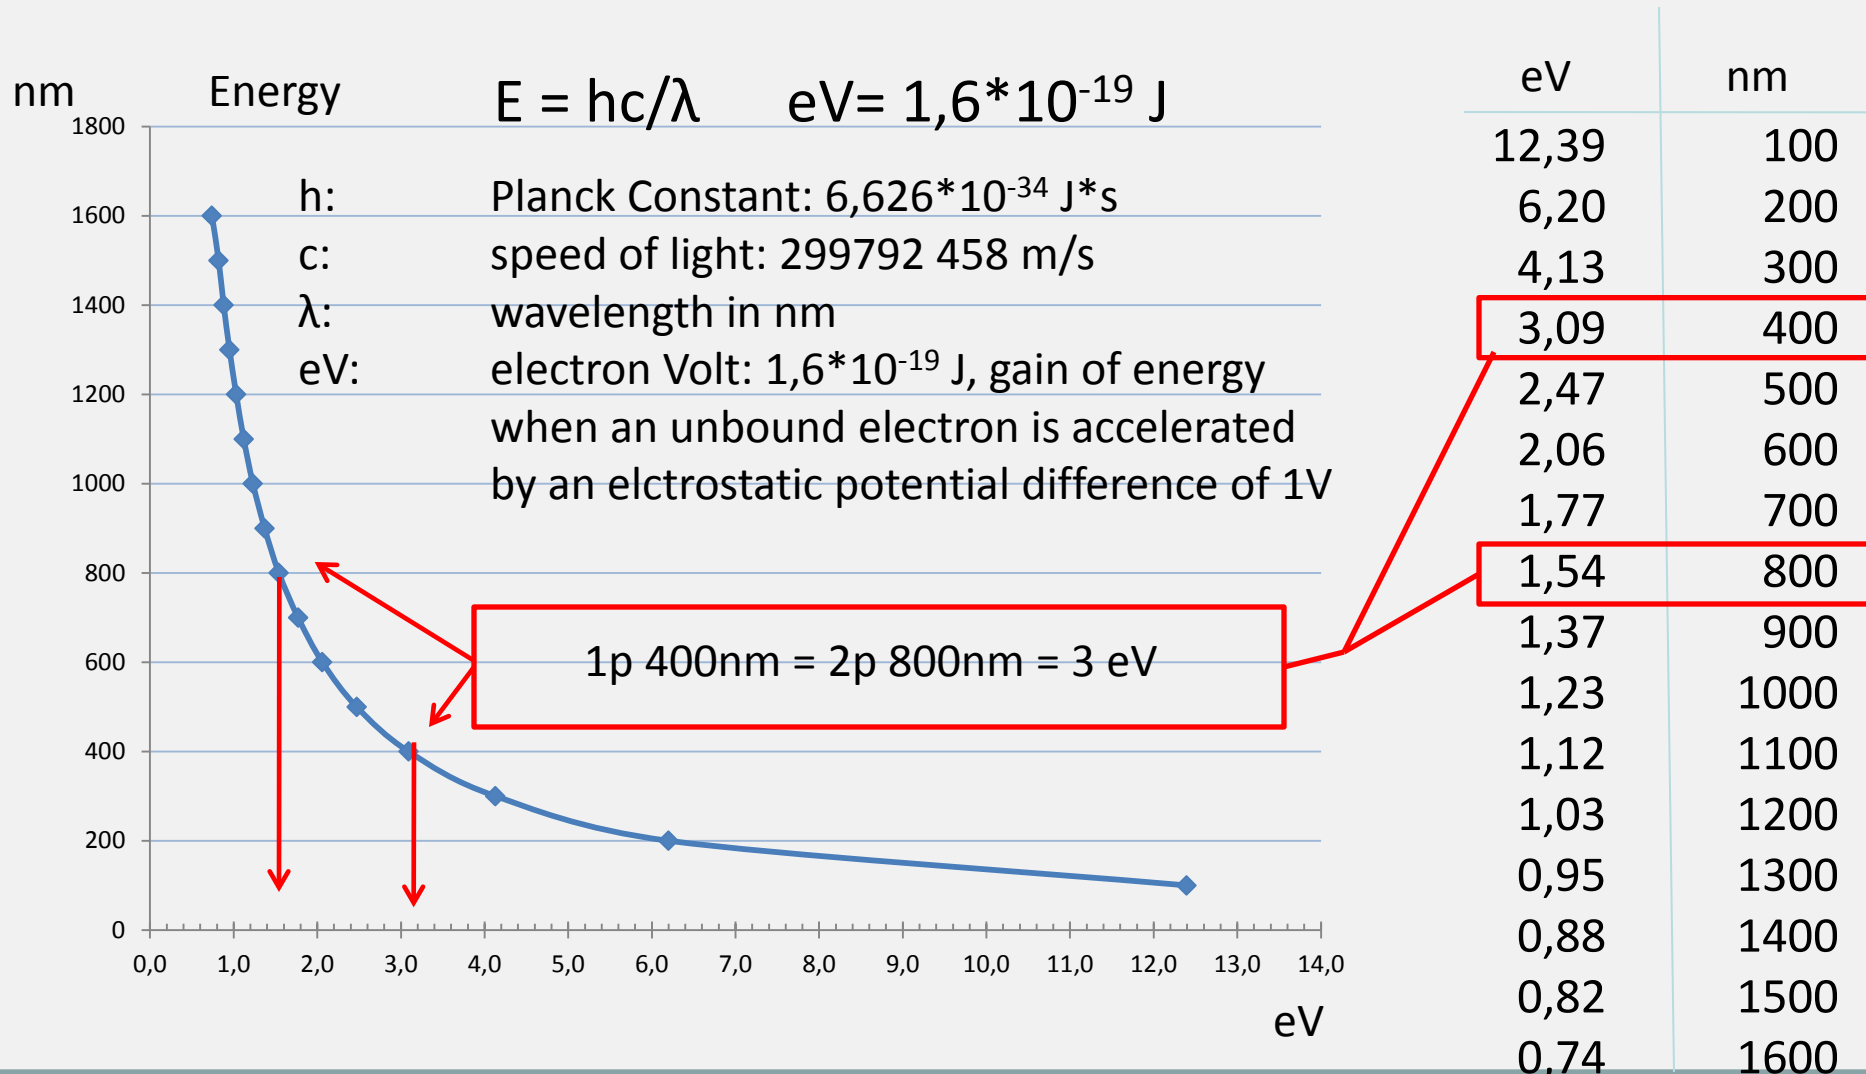



Theory for 2PM : How to excite (Tryptophan)

Single-photon
 1 photon, 280 nm
 4.5 eV
 No laser for this...

$$\frac{A}{B} = \frac{8\pi h \nu^3}{c^3}$$

Two-photon
 2 photon, 580 nm
 2.13 eV x2
 4.26 eV


Three-photon
 3 photon, 840 nm
 1.47 eV x3
 4.41 eV

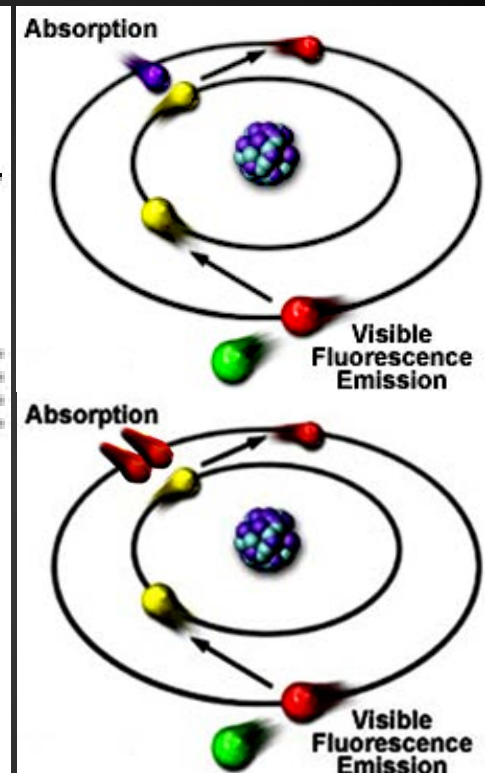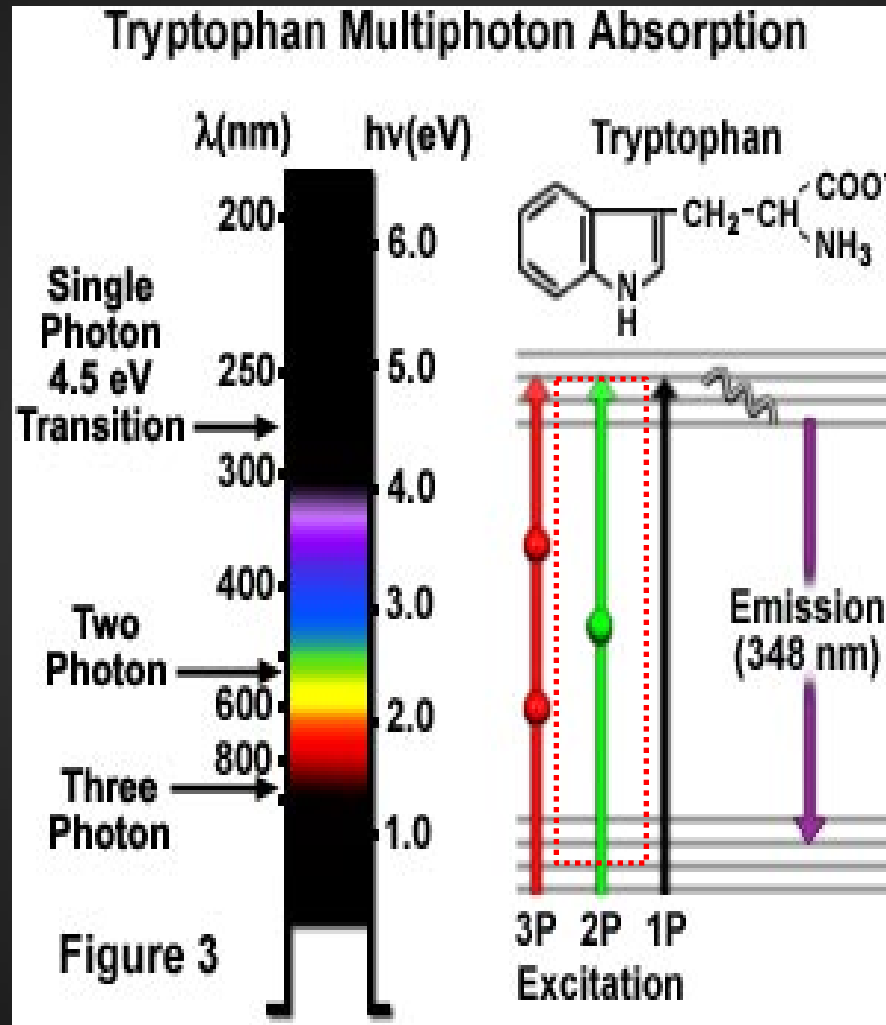

virtual state
 VERY short
 0.01 fsec
 (10⁻¹⁷ sec)

*2-PM hypothesis introduced by
 Maria Göppert-Mayer, doctoral thesis 1931*

Theory for 2PM : $\lambda \sim E$ - The Energy of a Photon

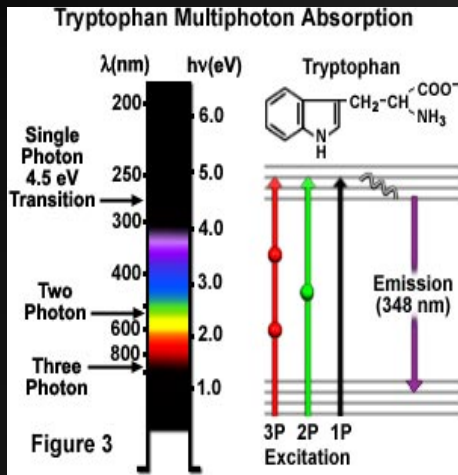

Fluorochrome	Absorption	Emission
Alexa Fluor 350	720-800	440
Alexa Fluor 488	720-800	515
Alexa Fluor 546	720-840	569
Alexa Fluor 568	720-840	596
Alexa Fluor 594	720-850	610
Alexa Fluor 633	720-900	647
AMCA	780-800	444
bis-MSB	680-750	420
Bodipy	900-950	512
Calcium Crimson	900	615
Calcium green	780-850	531
Cascade Blue	750-800	420
Coumarin 307	780-800	530
CY2	780-800	506
CY3	780	565, 615
CY5	780-820	670
Dansyl Hydrazine	700-750	440


Near Infra Red

Observe: range of overlap of potential Excitation
760nm : excite A488 & A633 *

for multicolor 2PM choose fluorophores so that they do overlap in excitation BUT NOT emission



* has to be checked on microscope

Dealing with fluorescence in 2P

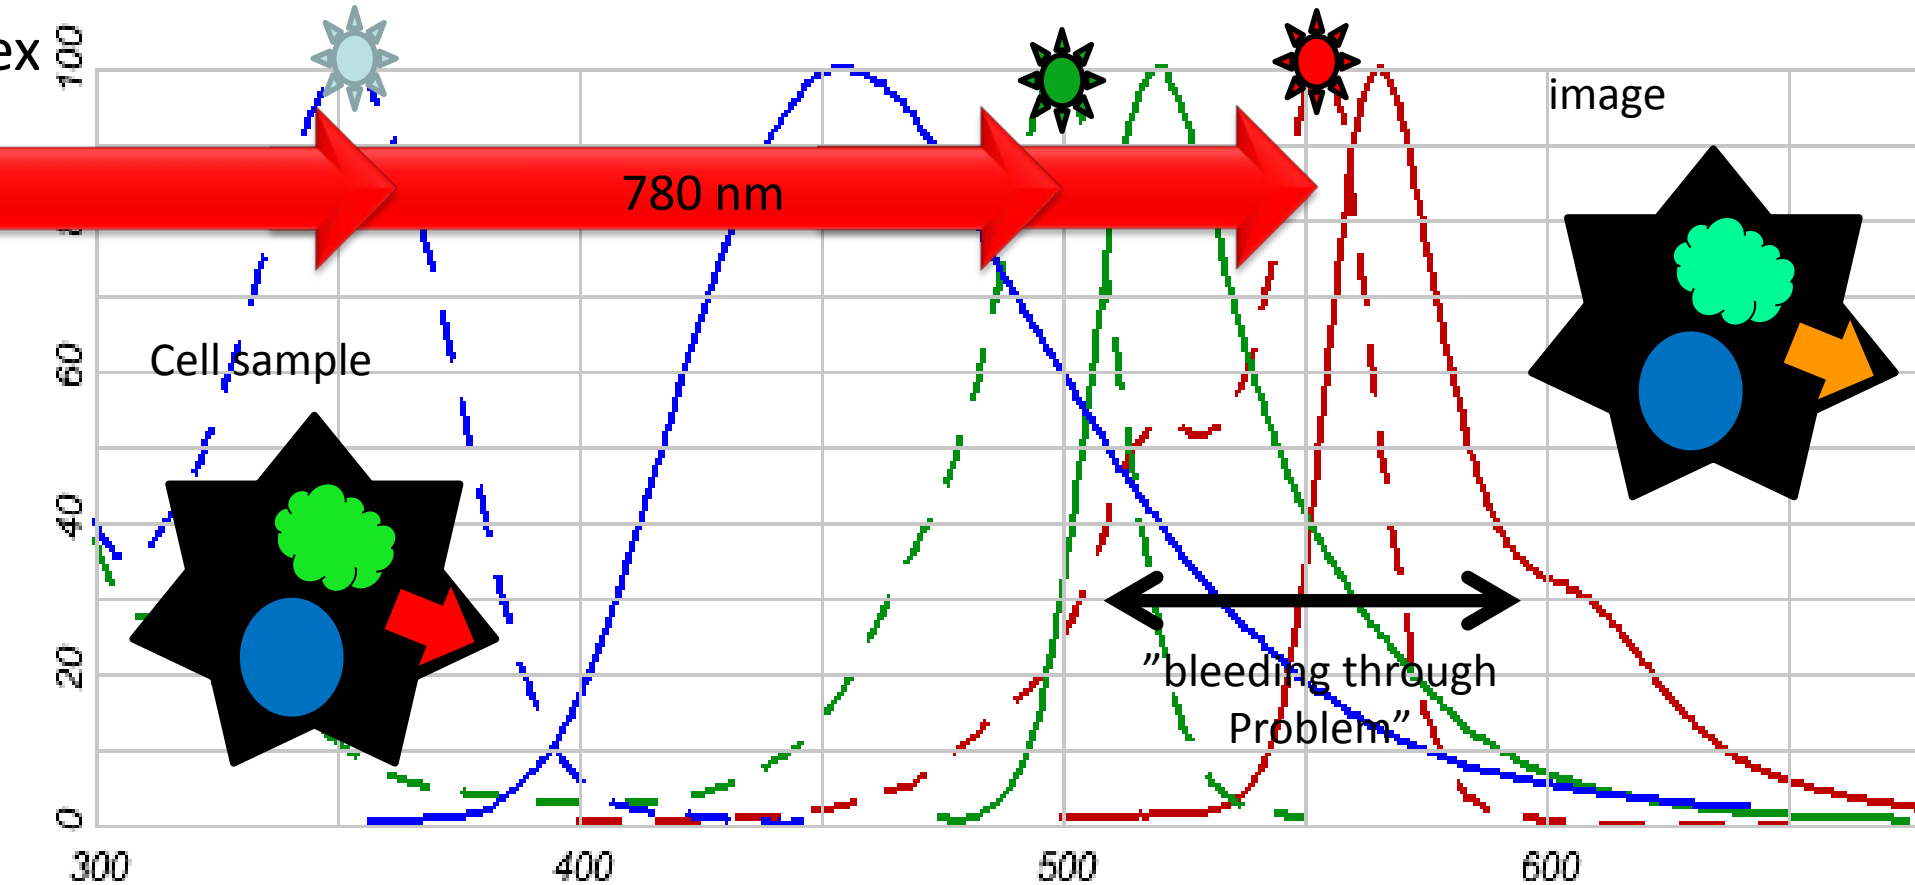

The 780nm NIR Laser might/will excite all three fluorophores, the Instrument has to unmix the mixture of Blue/Green/Red, or we have to use better fluorophore combination


Reminder – simultaneous vs sequential scanning

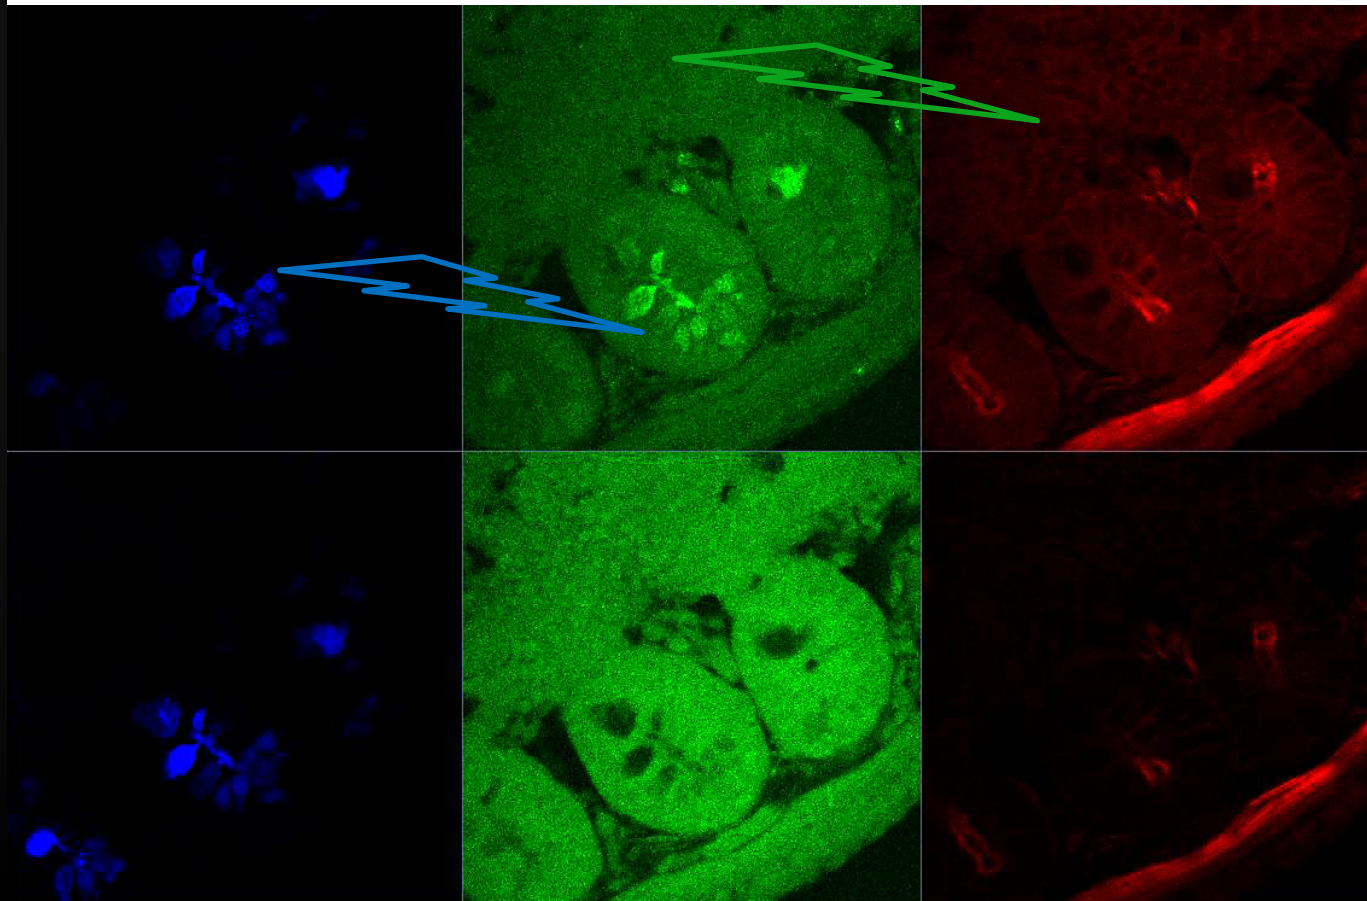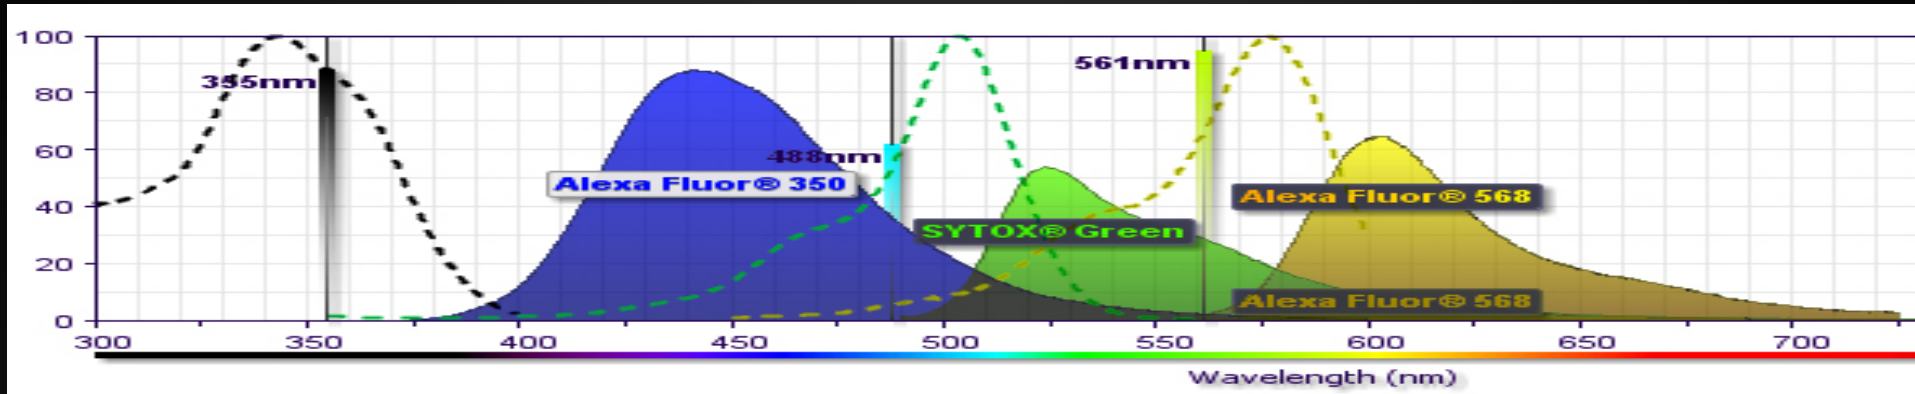

Simultaneous Excitation
Resulted in artifact
Due to bleeding through
on "green" image, where
the "blue" appears and
on the red image where
the "green appears"


Sequential scanning
Does not show such
Artifacts, therefore in
THIS sample the
Excitation are far
apart.

Multicolor imaging in 2P


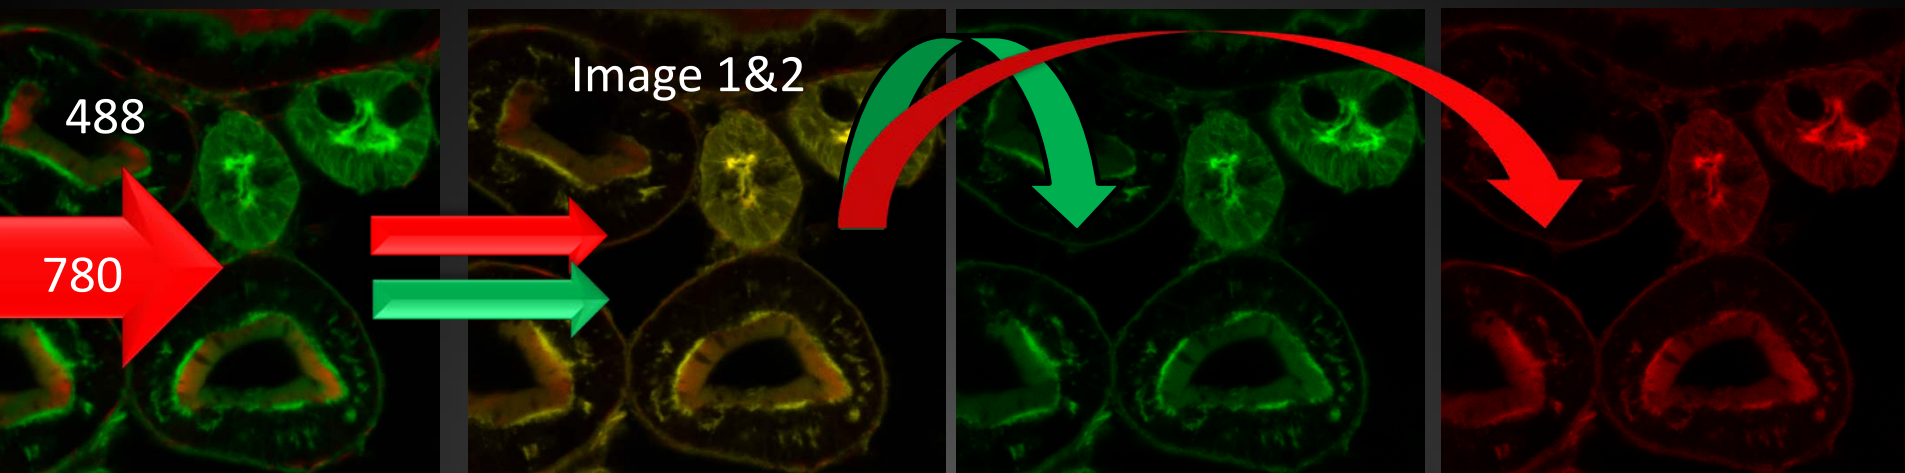


Simultaneous scan excites several fluorophore at once, emission is guided by filter and beamsplitter to PMTs. If FL-green bleed over into PMT of FL-red it will be seen here (in red). Sequential scan excites and collects one fluorophore at a time.

! Be sure that 488 does result in emission of FL red in the "green range"... Test that...

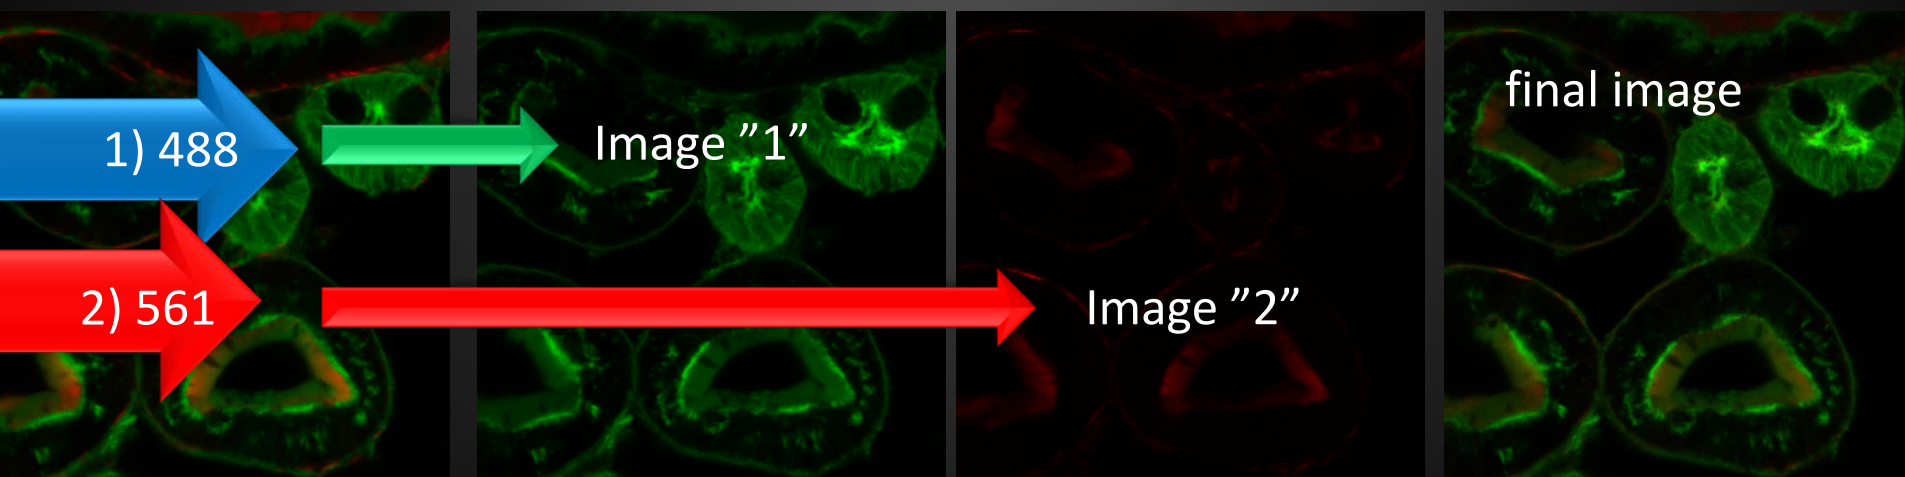

Lambda Scan with LSM – linear unmixing

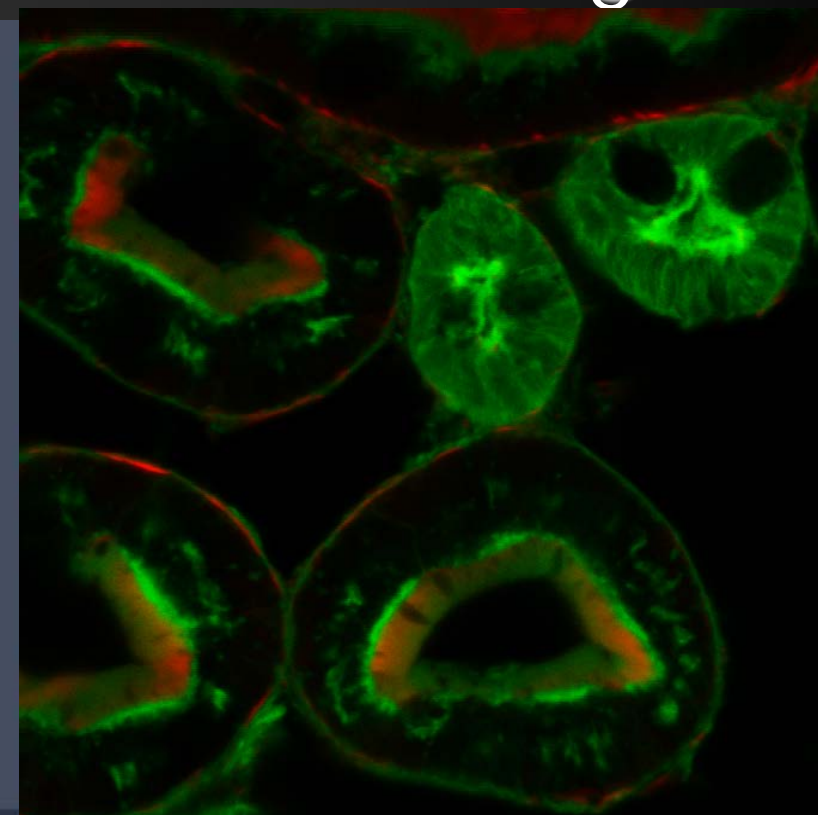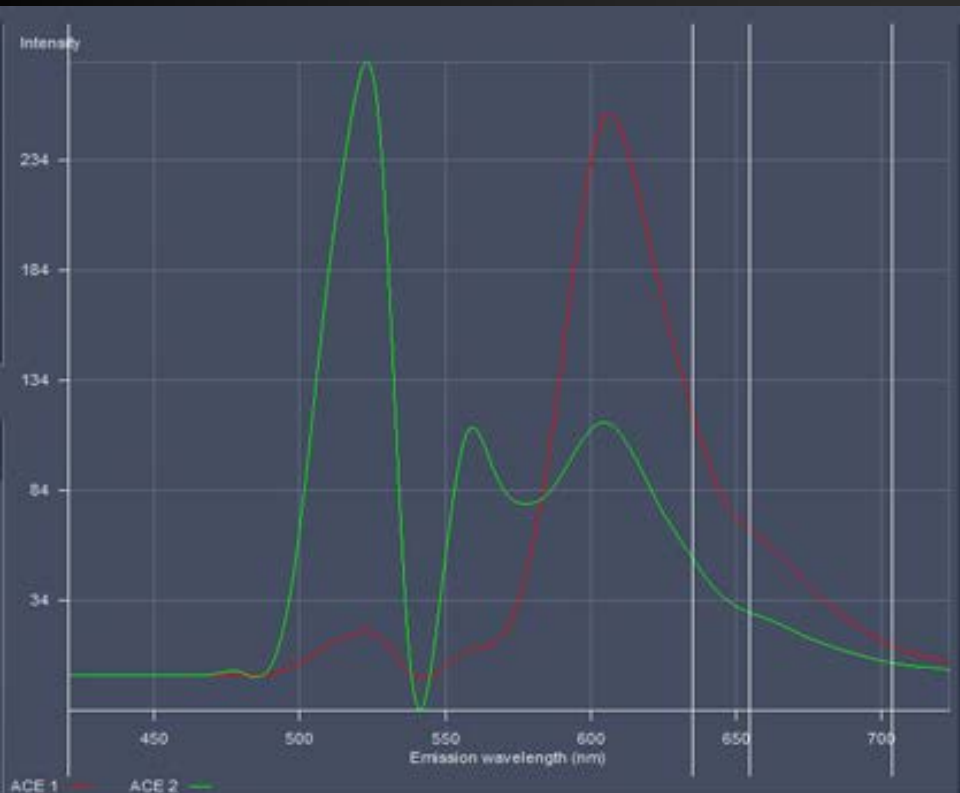

Emission wavelength [nm]
420
430
440
450
459
469
479
489
496
508
518
528
537
547
557
567
576
586
596

ACE 1	ACE 2
0.0	0.2
0.0	0.2
0.0	0.1
0.0	0.1
0.0	0.1
0.0	0.2
0.0	1.7
0.0	1.5
4.2	50.5
12.7	163.9
18.6	255.0
17.1	243.7
0.8	10.6
1.5	25.0
11.0	109.3
14.8	92.4
39.0	77.9
105.1	83.5
200.1	104.4

Linear Unmixing determines the relative contribution from each fluorophore for every pixel of the image. And recalculates an image for Fluorophores used

WHY USE 2P?

- to see deeper



Nikon instruments

See deeper – scattering problem

NIR light : 700-1100nm travelling through Specimen to focal plane will not scatter and disperse* as much as light of shorter λ (350-633 nm for FL microscopy)


➤ excitation of fluorophores in greater depth

Problem: different fluorophores need its own NIR Laser?

Solution: Laser can be tuned from e.g. 690 to 1040 nm, fluorophores have wide excitation range in 2PM

*(due to different refractive indices of the various components in specimen)


See also :
Optical Clearing

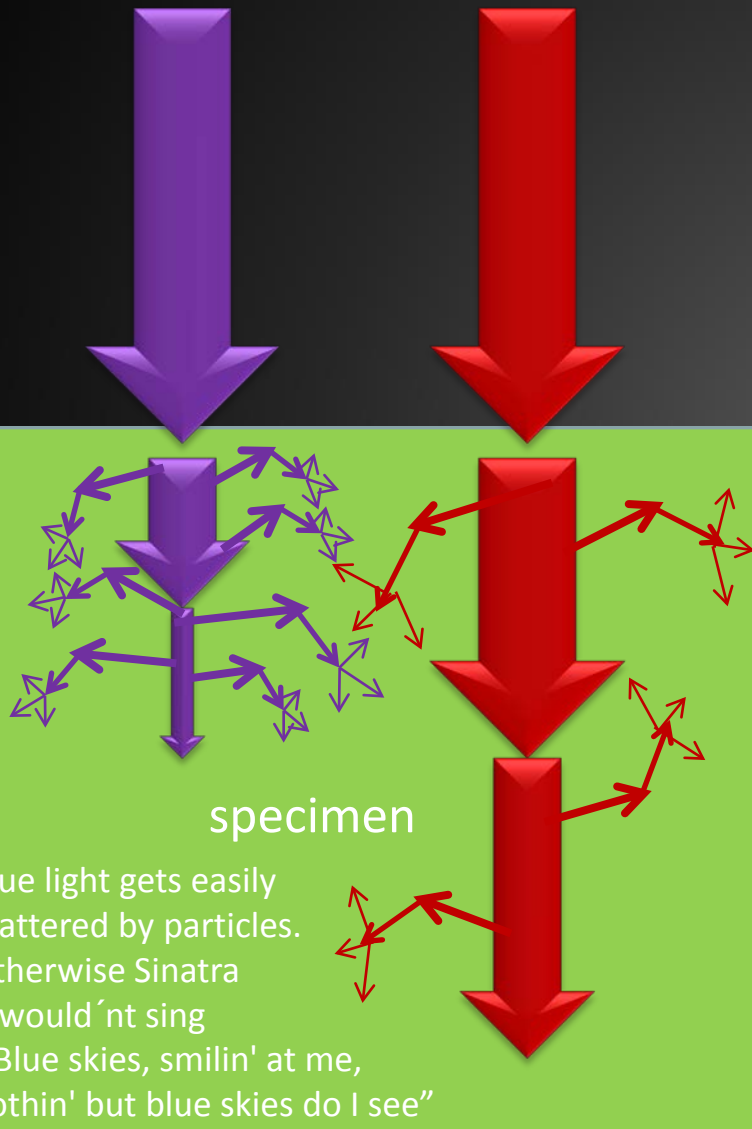

specimen


Blue light gets easily scattered by particles. Otherwise Sinatra c/would´nt sing "Blue skies, smilin' at me, nothin' but blue skies do I see"

See deeper – absorption problem

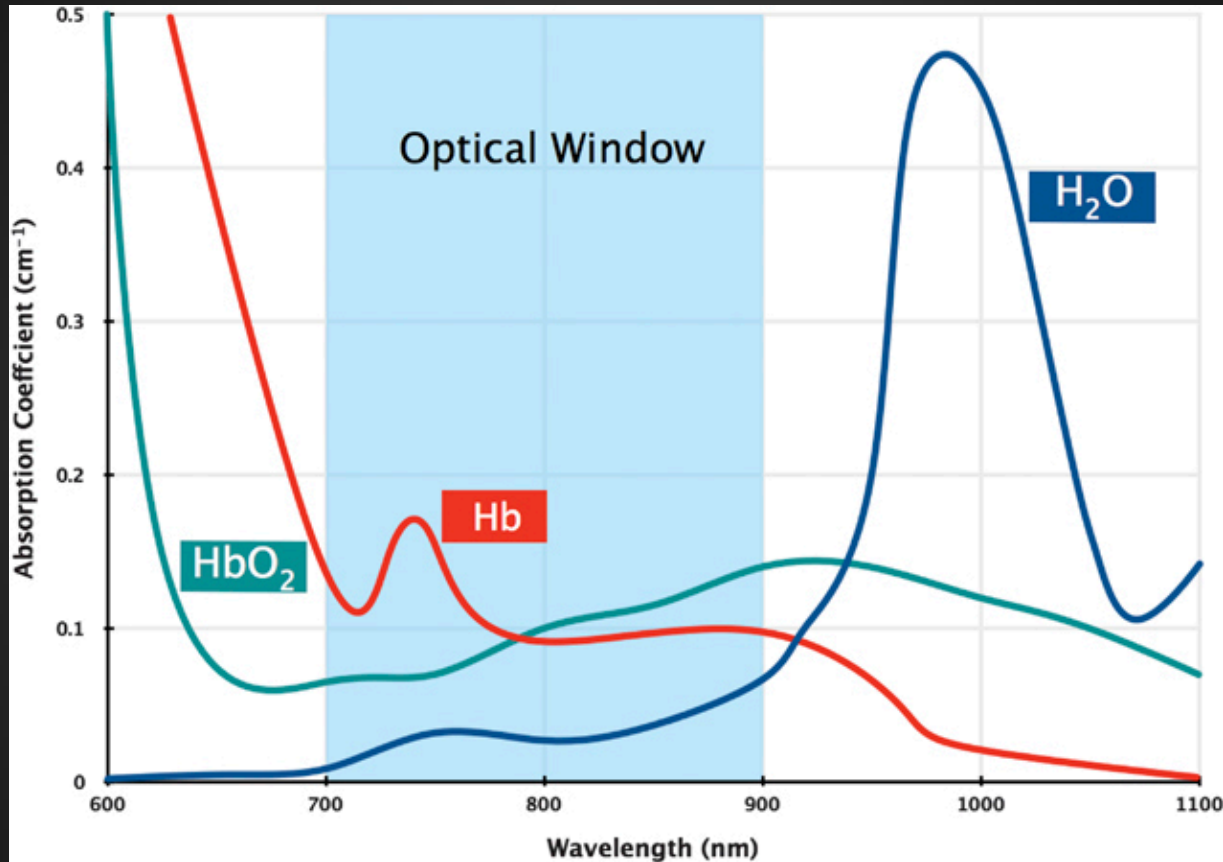

Tissue optical window: 700nm-900nm
(absorption of hemoglobin/tissue component
and water)

See deeper

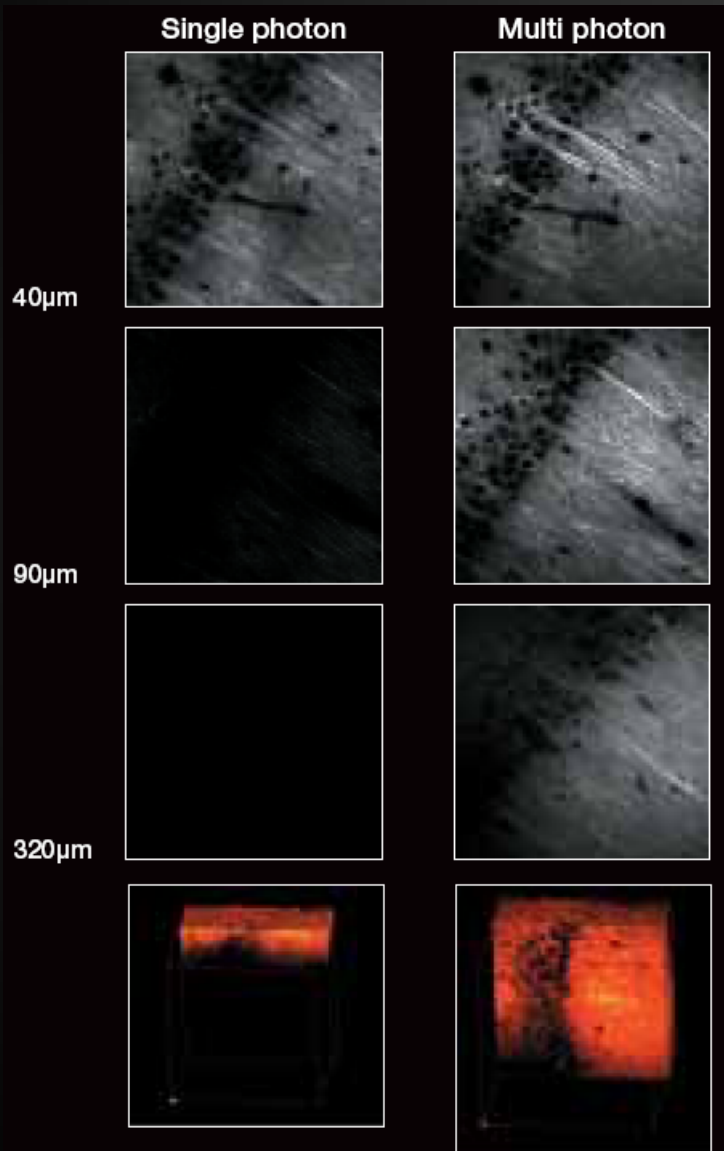

XYZ images of mouse brain sections expressing GFP, comparing single-photon 488 nm excitation and two-photon 910 nm excitation.

With single photon excitation, tissue can be observed only to a depth of about 90 µm, but with two photons, observation to a depth of about 320 µm is possible.


Items displayed in color are vertical cross sections of 3-dimensionally constructed images.

*Specimens provided by:
Kimihiro Kameyama, Tomoyo Ochiishi, Kazuyuki Kiyosue, Tatsuhiko Ebihara
Molecular Neurobiology Group, Neuroscience Research Institute,
National Institute of Advanced Industrial Science and Technology, Japan*

Brochure, OLYMPUS, FV1000MPE

WHY USE 2P?

- small excitation volume, no pinhole

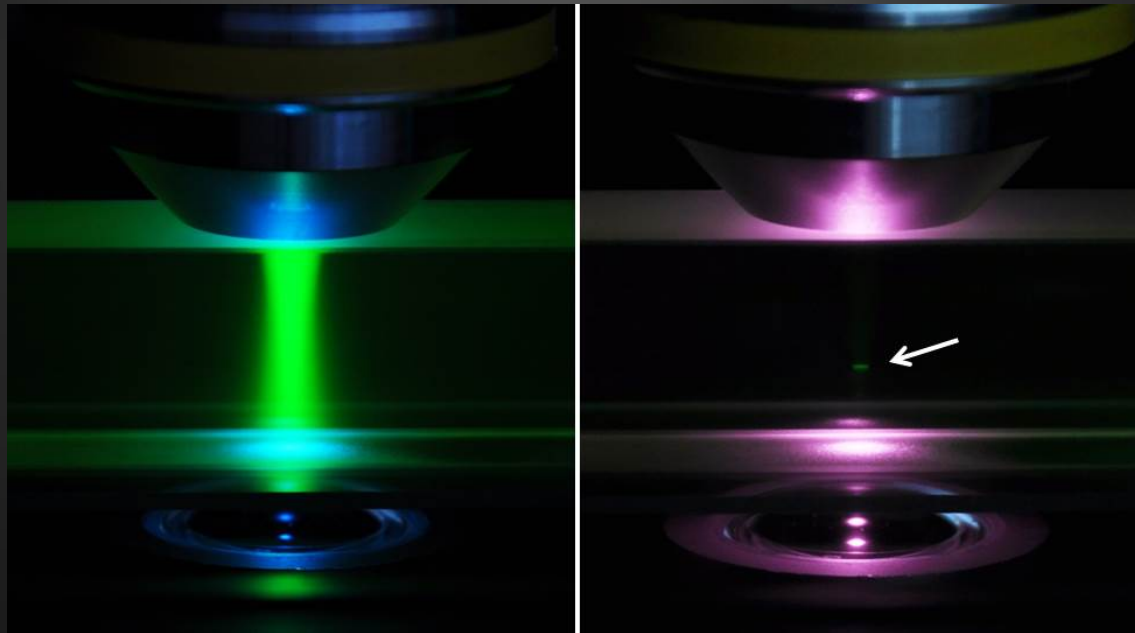


Matyas Molnar

Small focus spot

Multiphoton

LSM

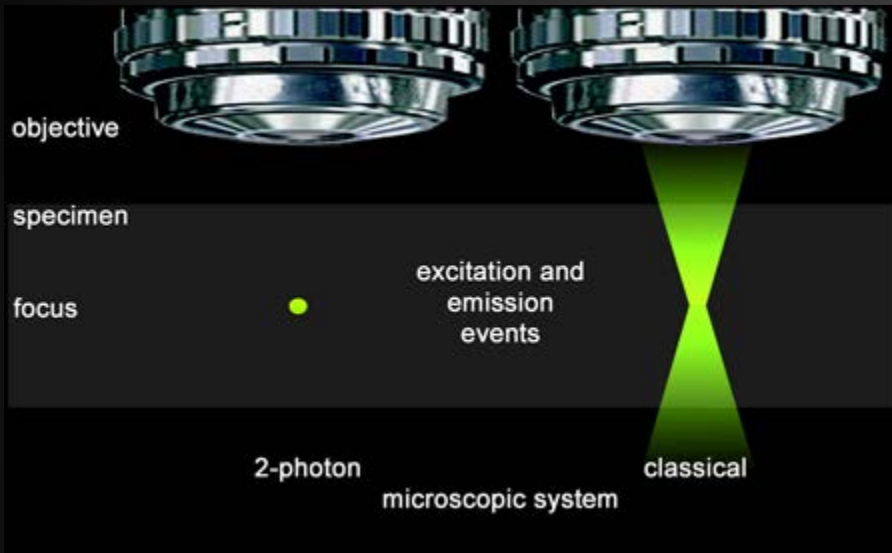

Two-Photon event occurs only in focus volume

➤ All emission light is directly from focus

Resolution is similar (or worse) to LSM

➤ $0.3 \times 1 \mu\text{m}$ ellipsoid (high NA objective)

Penetration depth depending on specimen and optical parameter but might be up to nearly 1mm

These features will be important for various live cell imaging techniques, like bleaching, photodamaging, uncaging ...

$$Ex \sim (P_{\text{avg}}/A)^2 = I^2$$

$$Ex \sim P_{\text{avg}}$$


That's why Multiphoton is also named Nonlinear.

Chance for 2PM event drops drastically with distance to focus

Small focus spot

Laser of LSM scans through specimen

Laser of 2PM scans through specimen

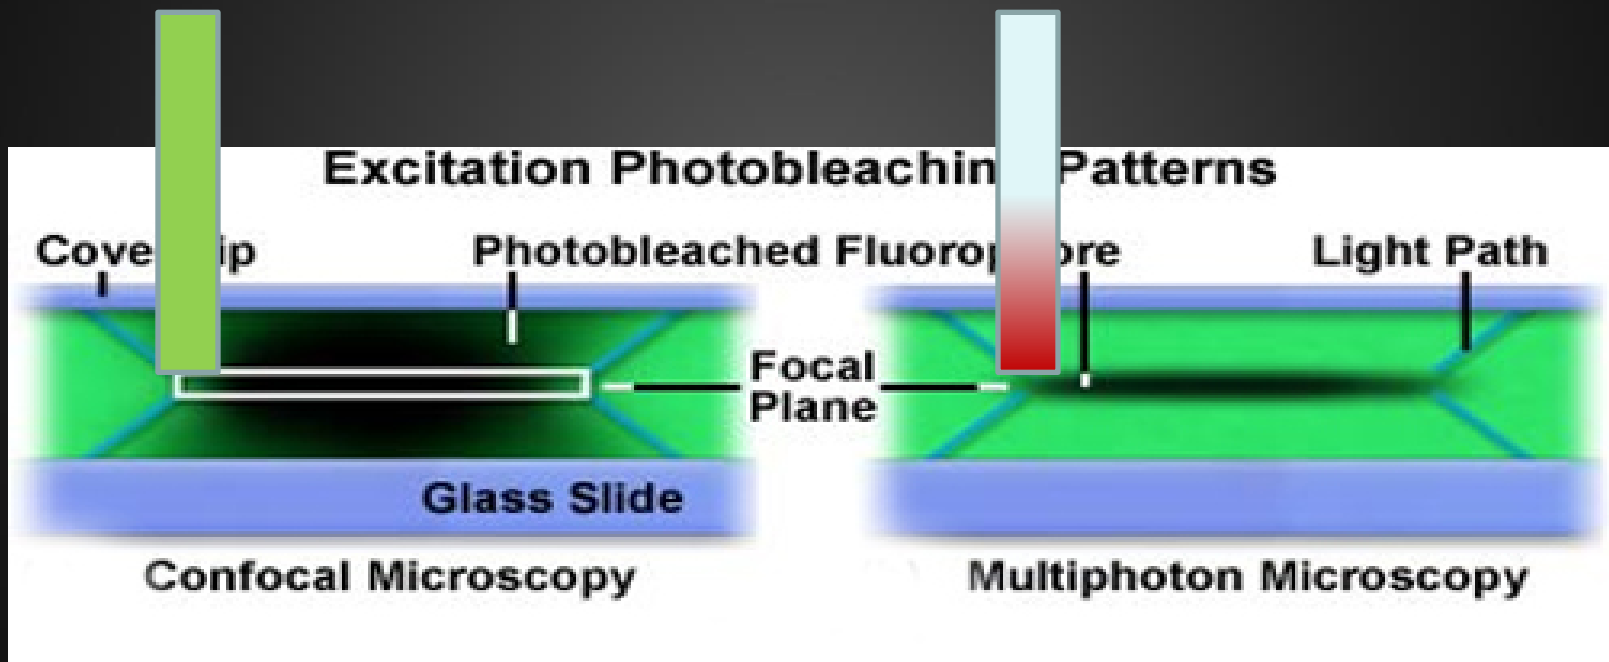

excitation/emission and photodamage/heat

occurs within specimen
also outside the focal plane

occurs within specimen
only in the focal plane

Small focus spot

What is the chance that 2 photons hit the same fluorophore at almost the same time?

- a matter of time and area
- **The probability of observing a two-photon absorption event on a bright sunny day is 1 per 10,000,000 years, whereas the one-photon absorption takes place every second**

Time → the virtual state

- Δt of intermediate virtual state = 10 attosec (10^{-17} s)
- 1 attosecond (10^{-18} s) is the time window
- light travels 3 hydrogenatoms within 1 attosec


Area → the fluorophore

- quite small target

Problem: Light can not travel faster than speed of light

Solution: More photons are needed (high density of photons)

We need a million times more photons than in single photon fluorescence and "good" objectives

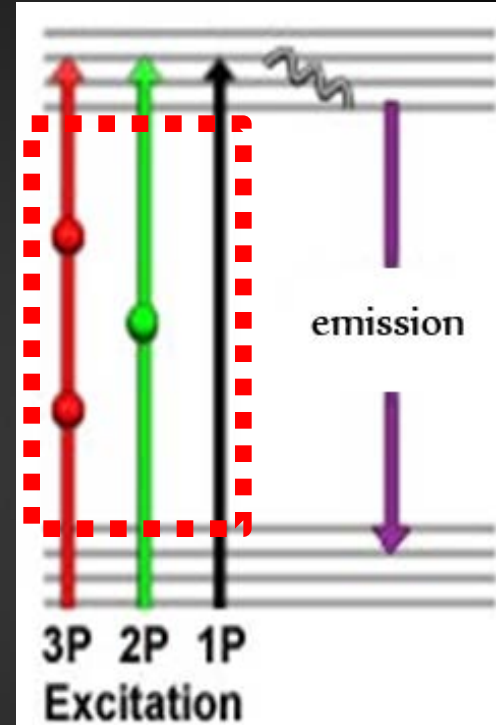

More photons please

Problem:

1 million times more photons? Very strong laser
There is no continuous wave laser to achieve this.

Solution: A moderate Laser with high photon intensity pulses


- low average power (0.3 - 2.5 W)
- high peak power (30-300 kW) pulses 50-100 fs wide
- pulse frequency 80 Mhz (1pulse/ 12,5ns)

This laser is dangerous when used (Class 4)!


Problem: Many fluorophores but one Laser

Solution: To excite a wide range of fluorophores the laser is tuneable for e.g. 700-1040 nm


Pulsed NIR Laser is tuneable for excitation wavelength twice the 1Photon-excitation wavelength

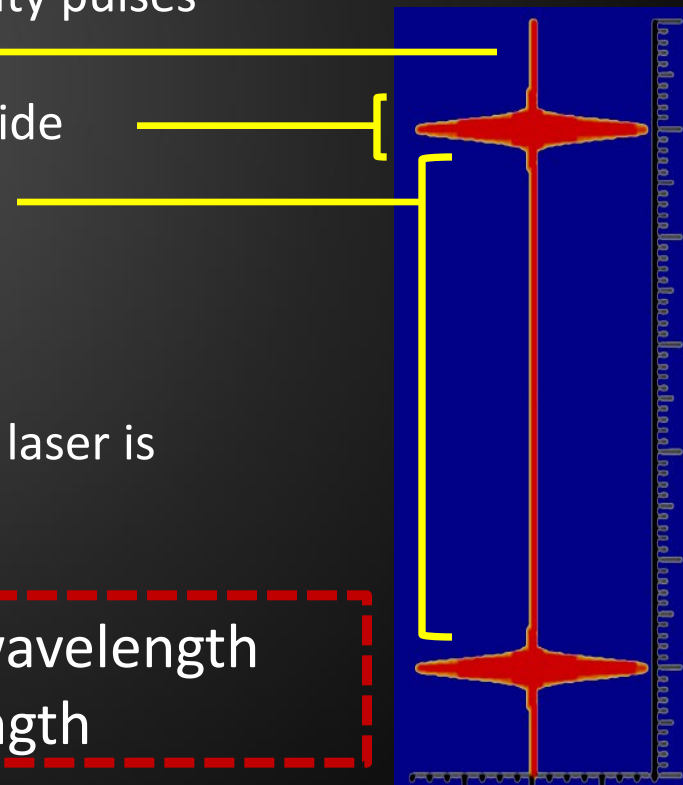

Principle of 2P excitation

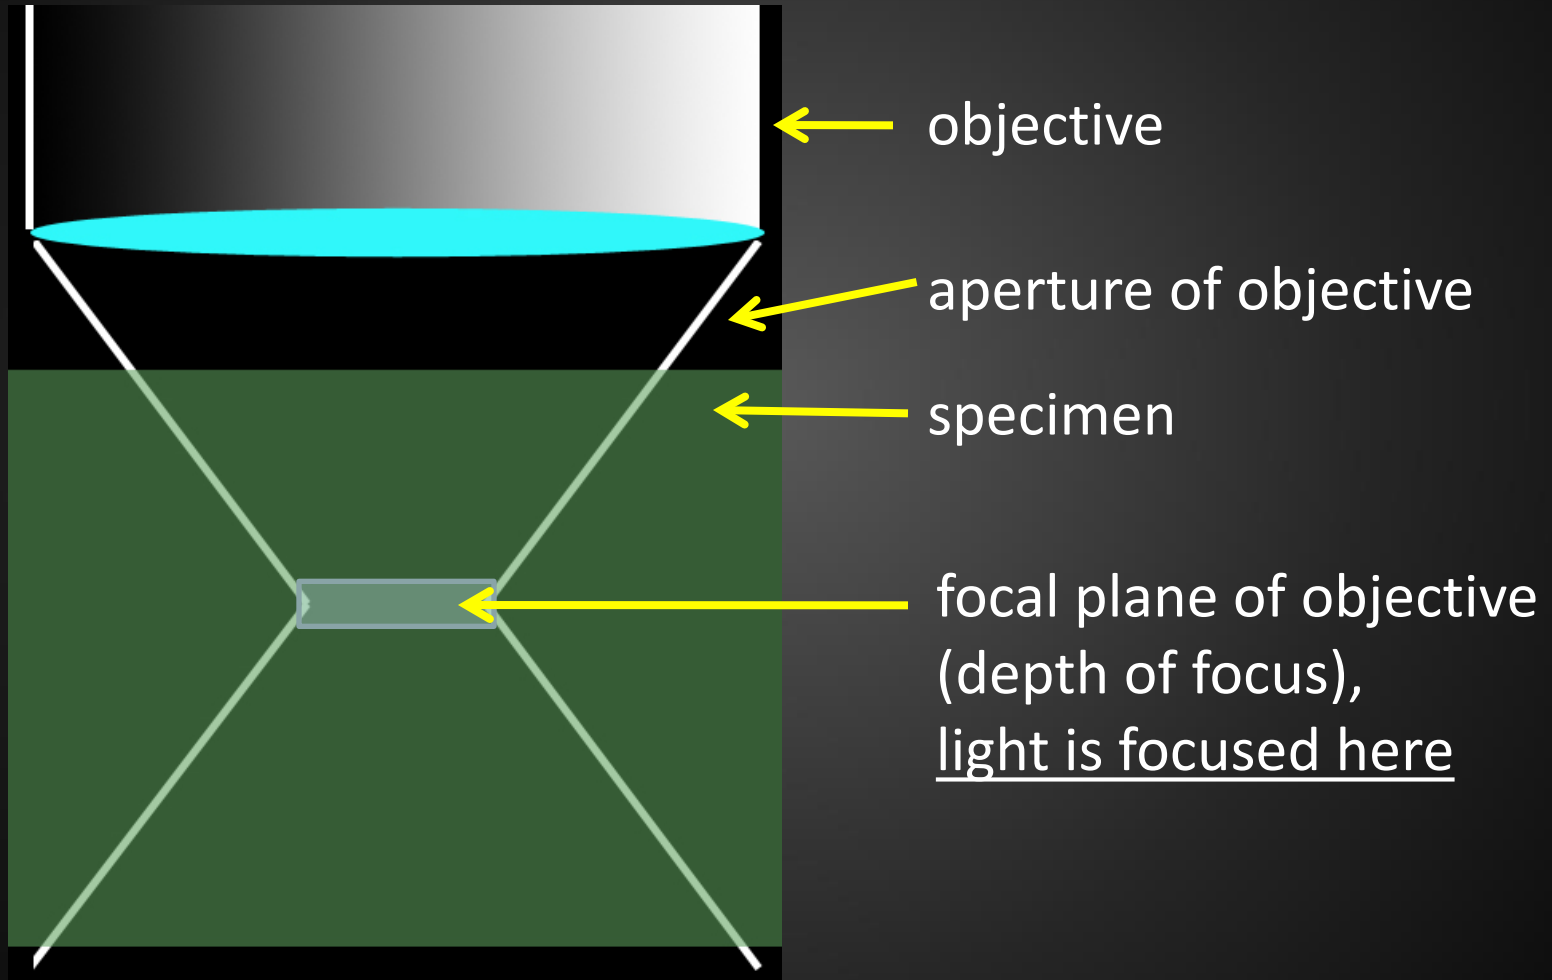


Principle of 2P excitation

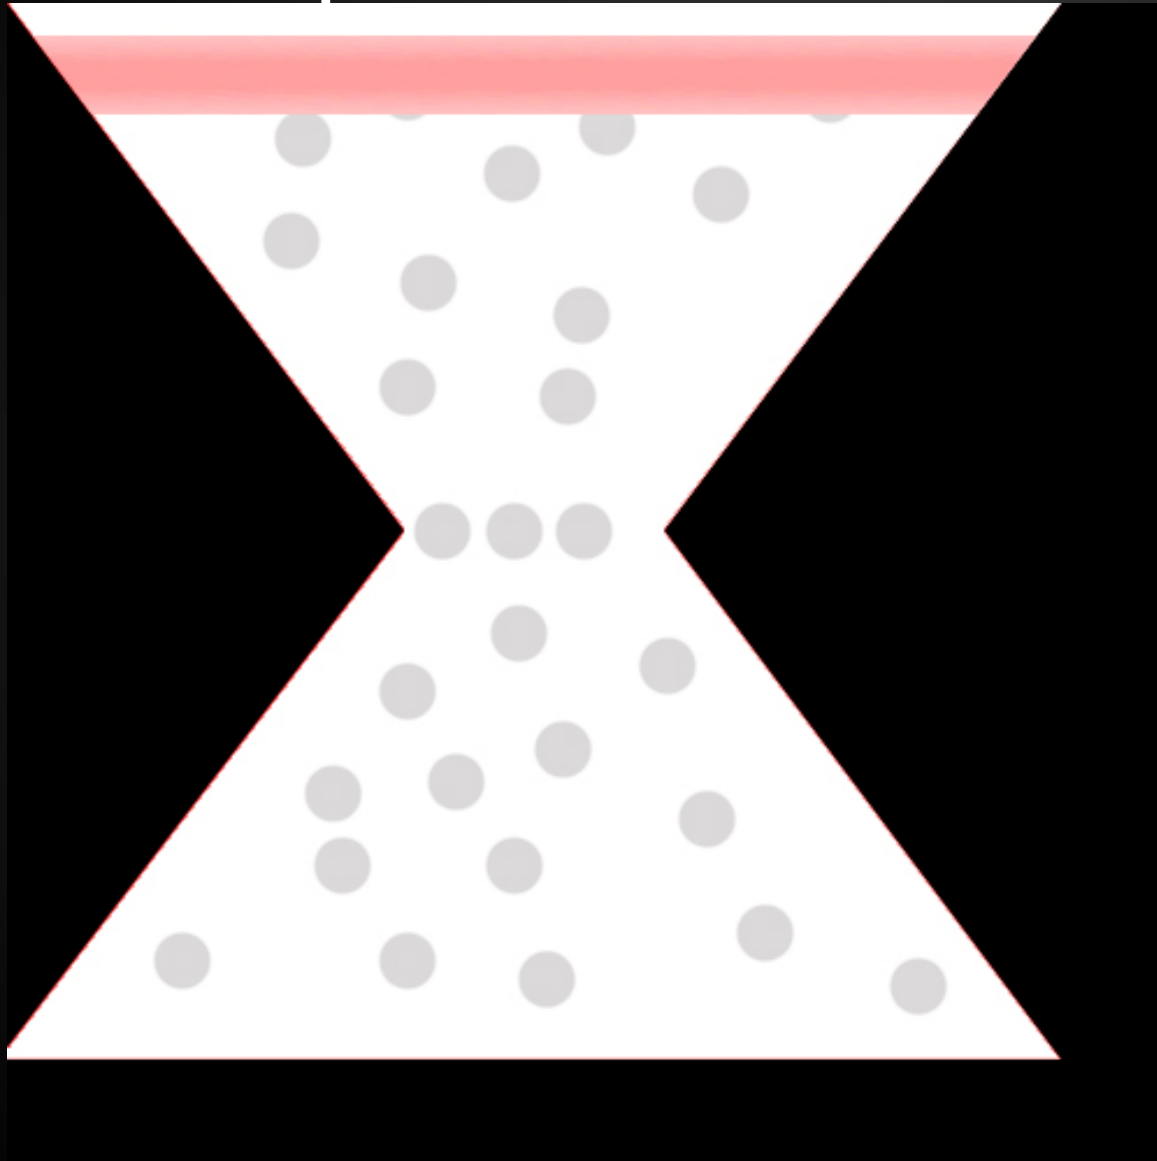


Laser pulse is far from focal plane, photon density is low, no chance for two photons to hit a fluorophore in one time

Principle of 2P excitation

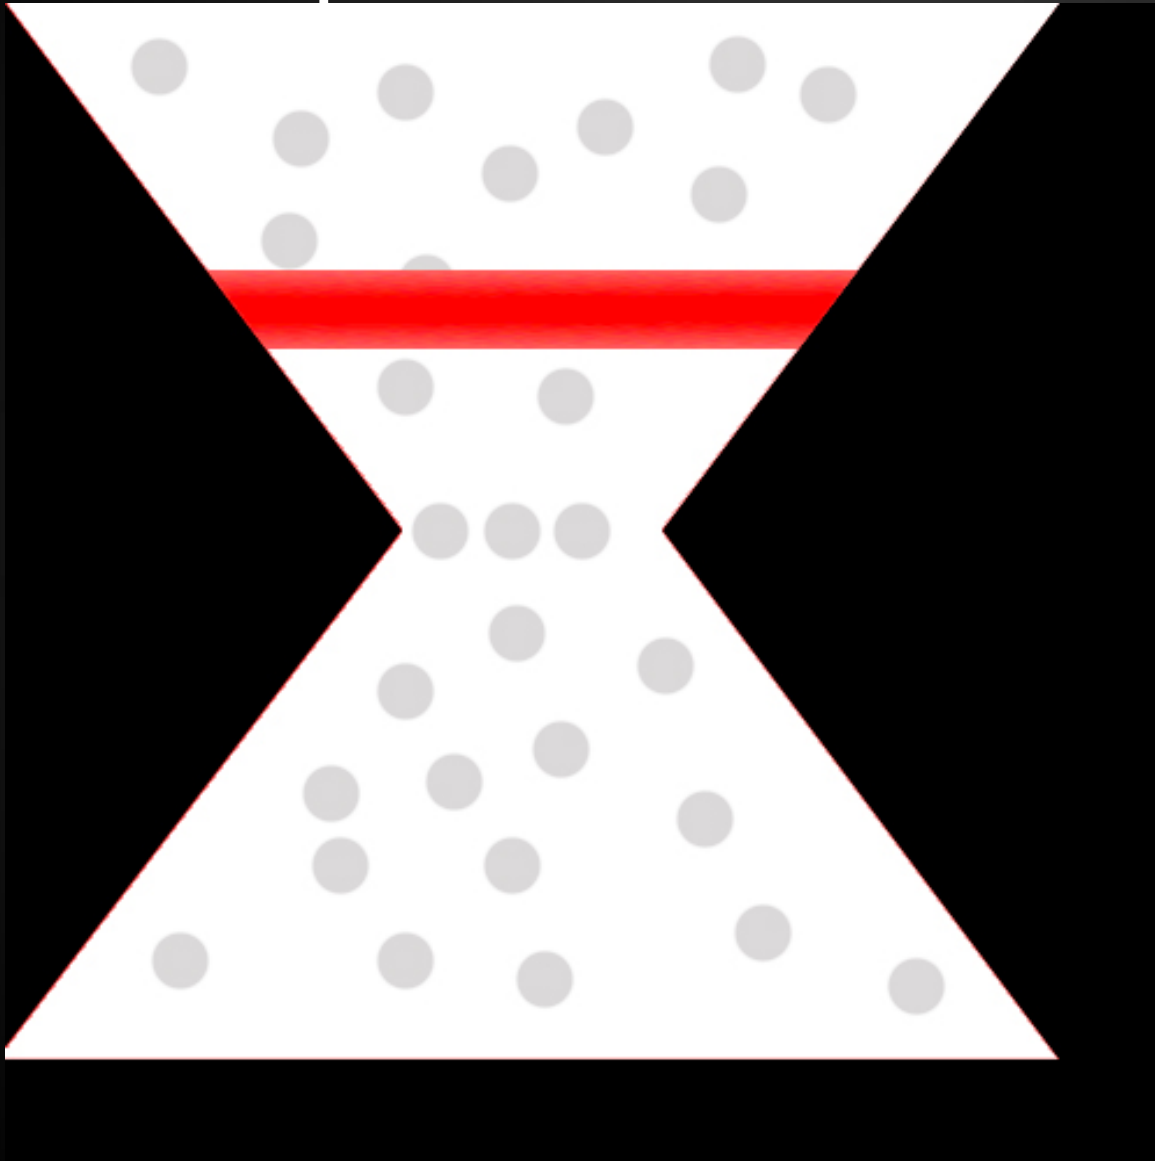


Laser pulse is closer to focal plane, photon density is more concentrated but still low, no chance for two photons to hit a fluorophore in one time

Principle of 2P excitation

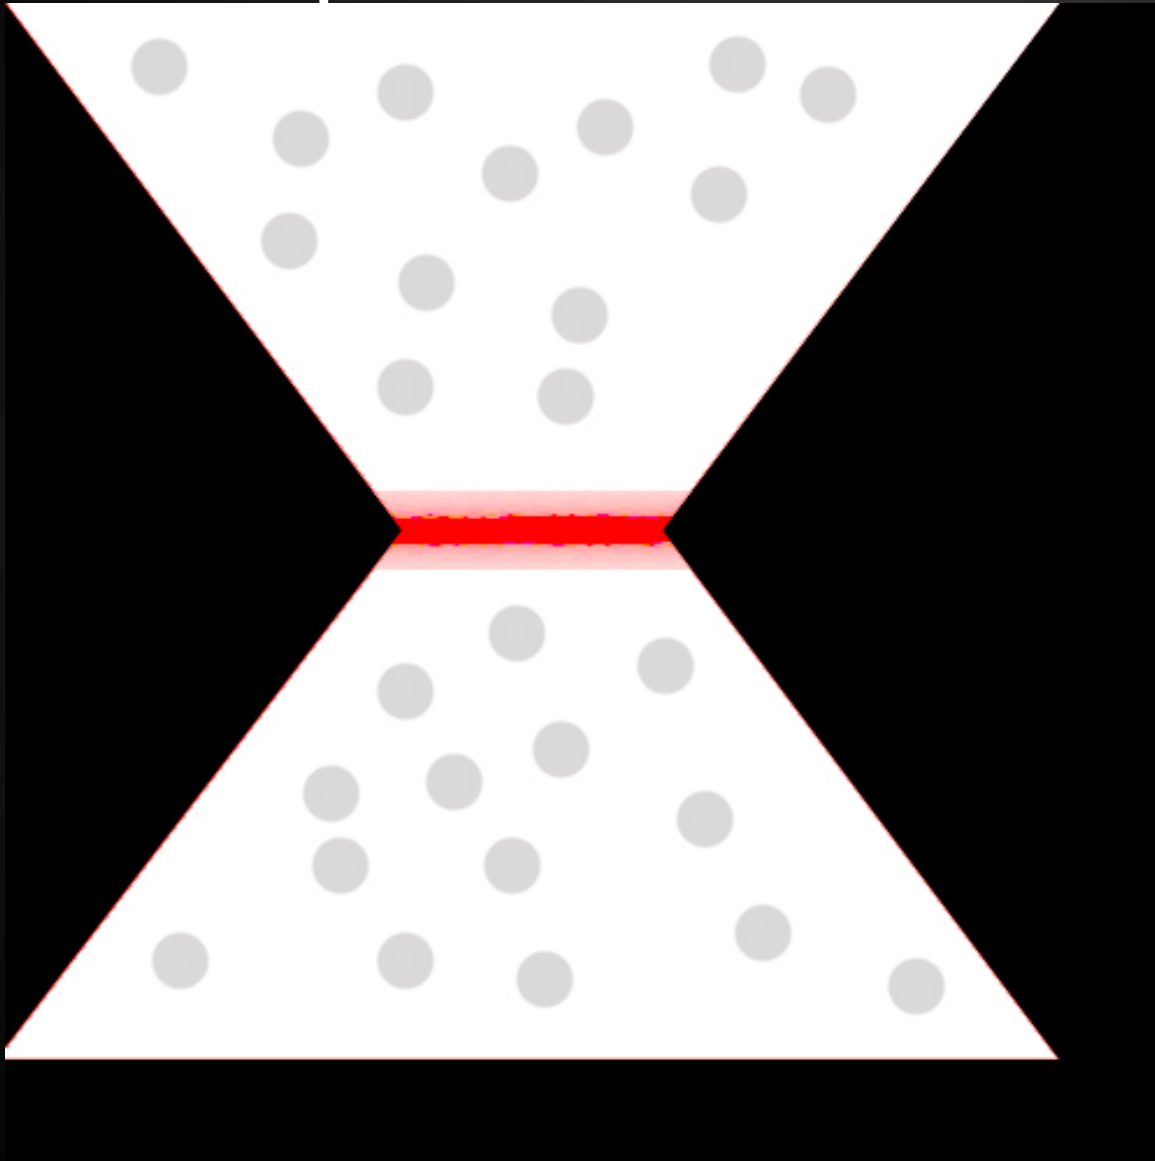



Laser pulse reached the focal plane, photon density is high, high probability for 2 photons to hit one fluorophore within 10 attosec

Principle of 2P excitation

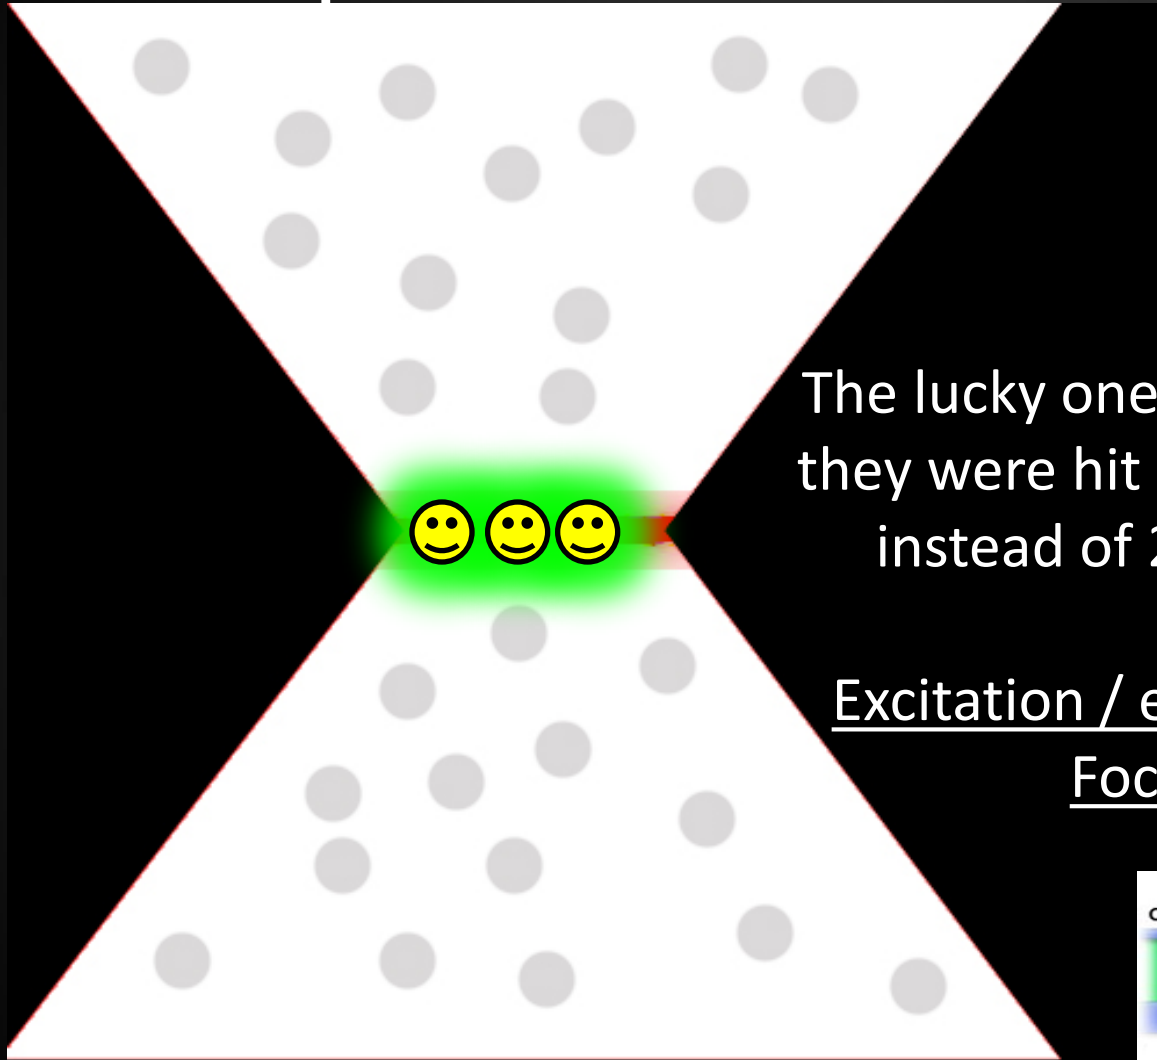


The lucky ones emit fluorescence like they were hit by 1 high energy photon instead of 2 low energy photons

Excitation / emission occurs only in Focal plane /spot

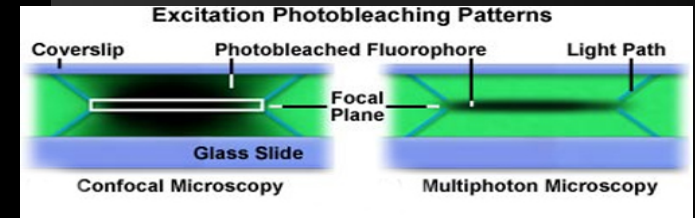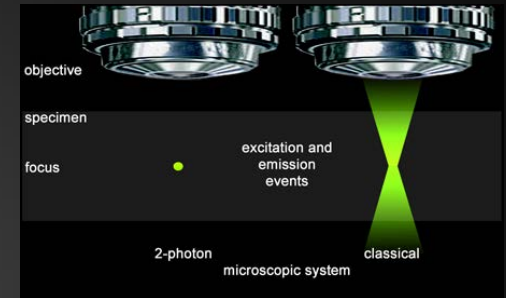


Principle of 2P excitation

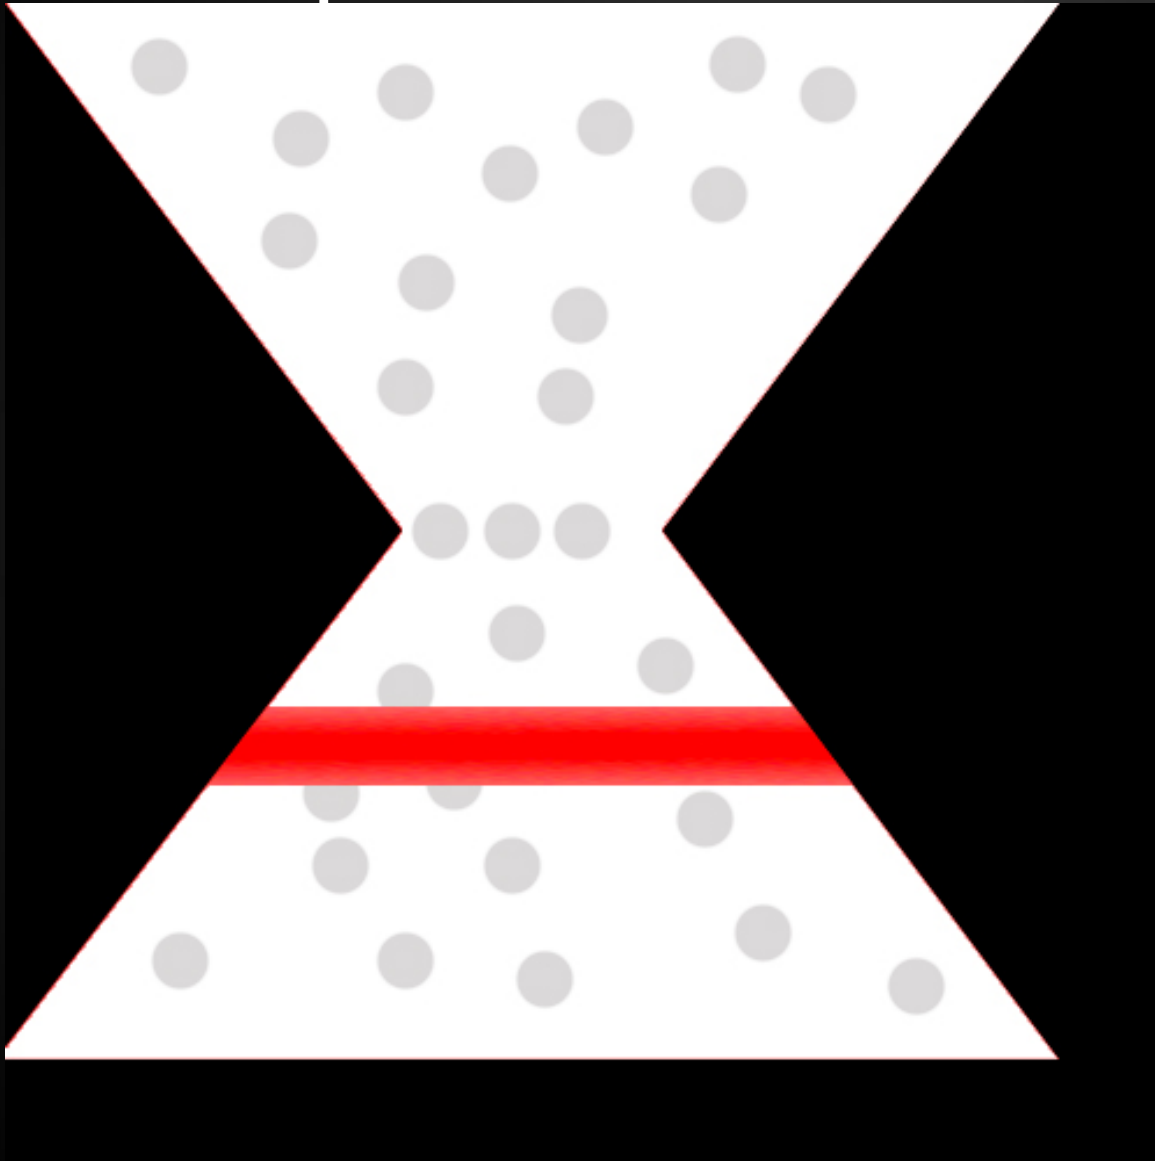


Laser pulse leaves focal plane,
NO incident of two photons hitting one fluorophore

Principle of 2P excitation

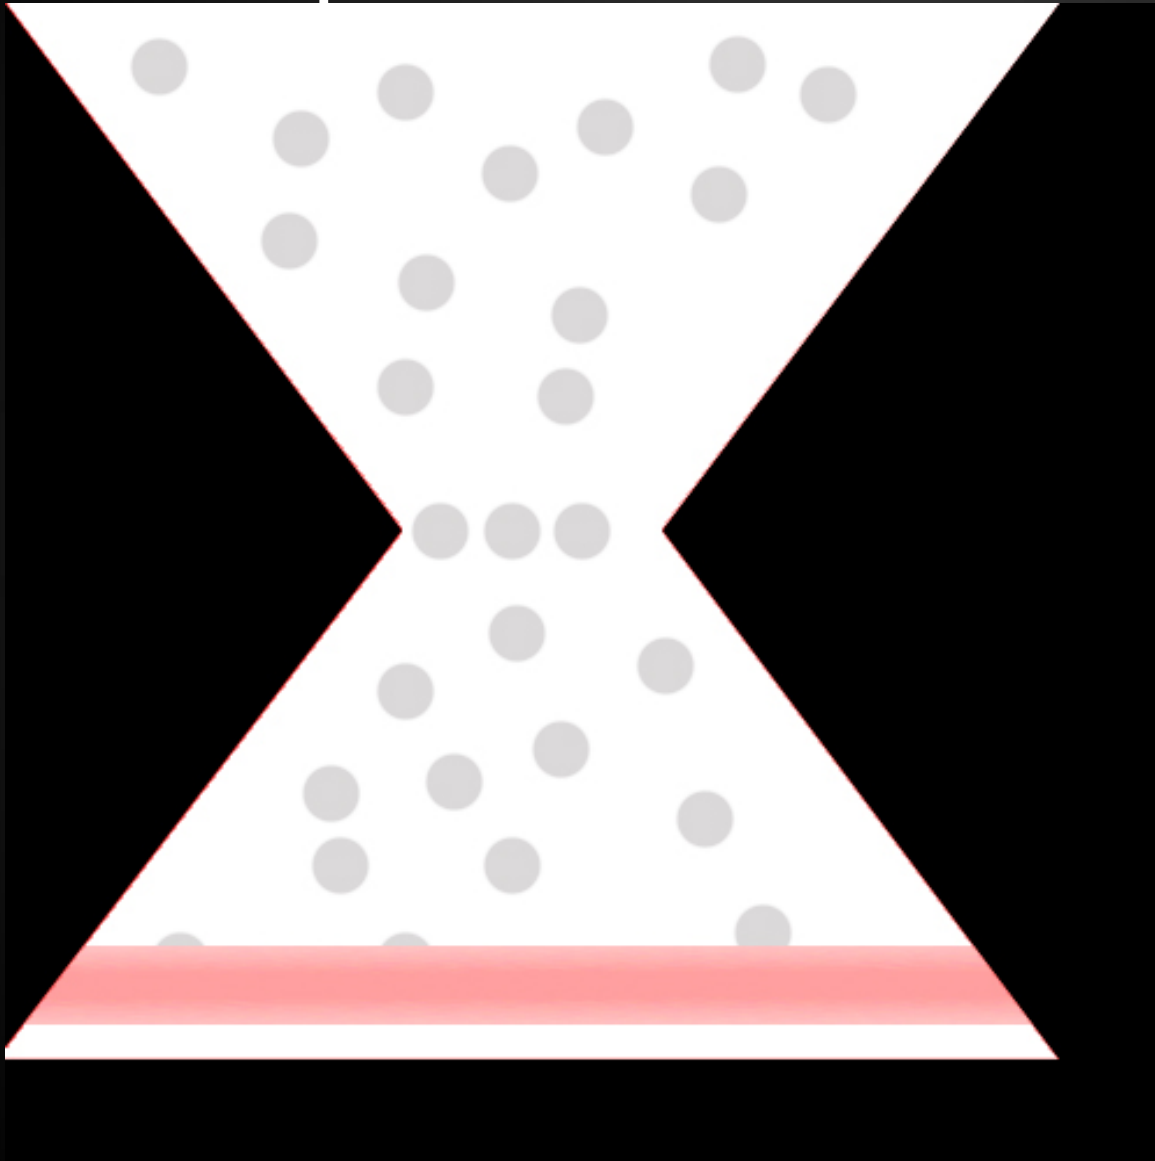

Laser pulse
disperses in tissue,
NO incident of two
photons hitting
one fluorophore

Principle of 2P excitation

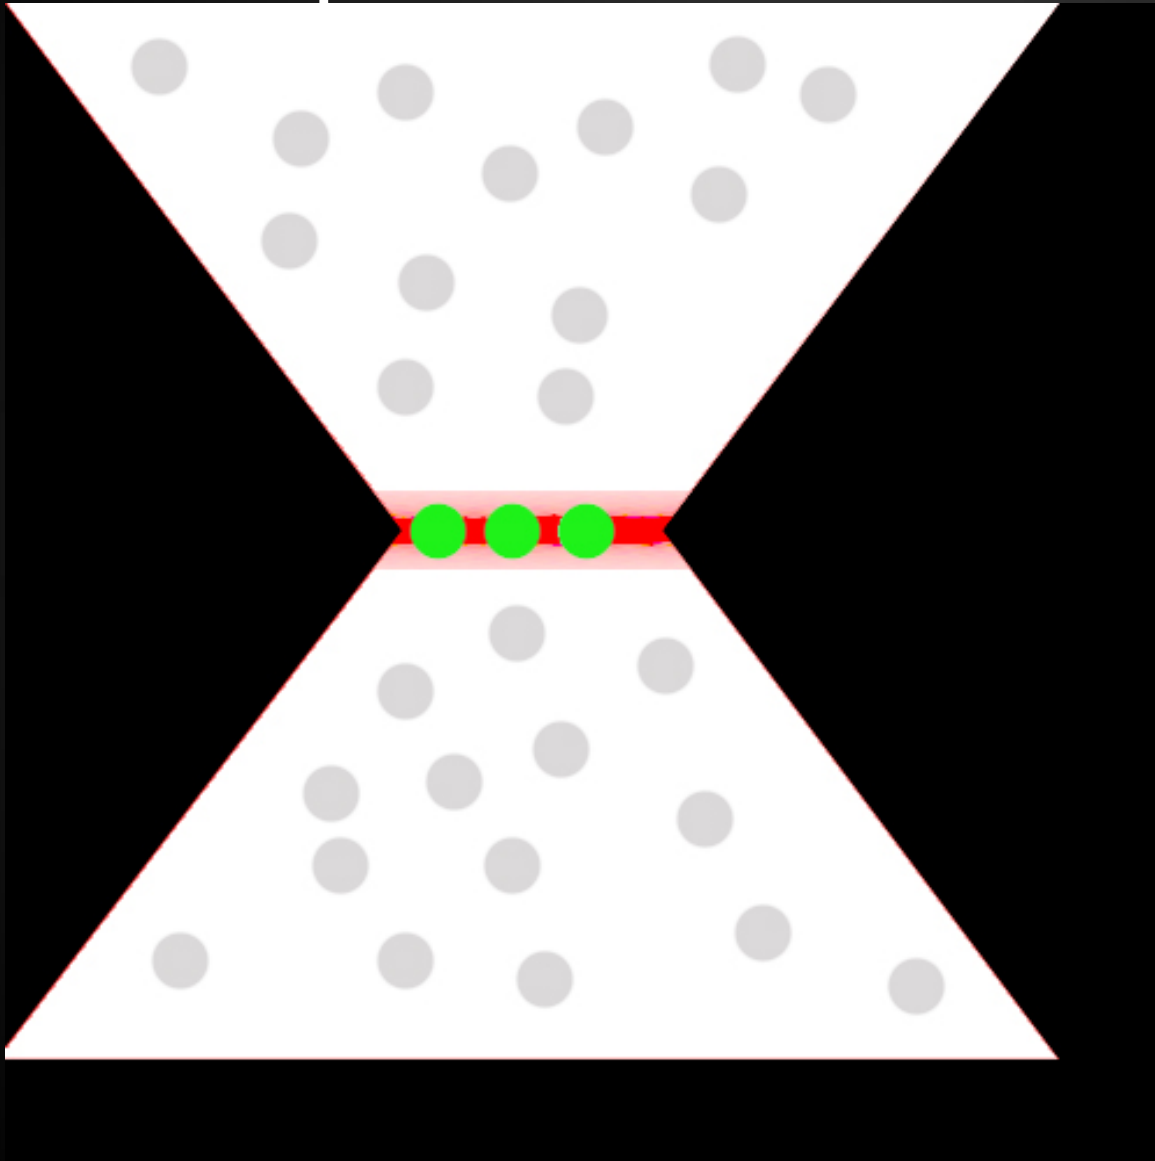

REMEMBER

Excitation / emission
occurs only in
Focal plane /spot
confocal image
without
a pinhole

Repeat again

Recapitulate:

- NIR Laser to reach deep
- Excitation of "normal" fluorophores via 2P effect
- NIR is tuneable over range e.g. 690 nm – 1040 nm
 - 2P is only happening in focal volume
- Ex/Em/photodamage only at focal volume

Applications:

Living animals

Manipulation of "precise" small volumes

Non-linear effects


Relax...

Light travels 300.000.000 m / s
→ 7.4 x around earth in one s
(40.075 km circumference)




But only 300 nm in one femtosecond
Or 30μm within 100 fs

The Femtosecond Laser:
Pulses of 100fs
1 fs = 1×10^{-15} sec

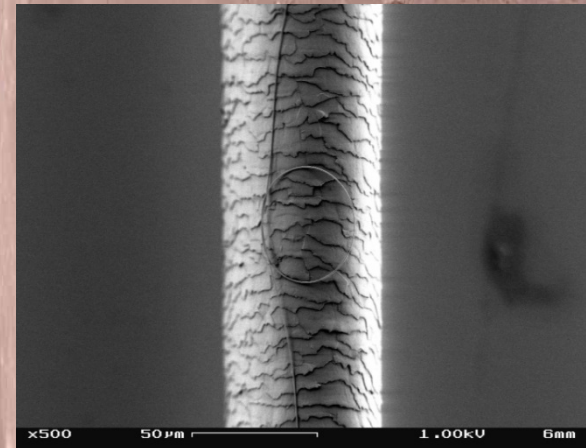

circumference of
human hair
53-565 μm

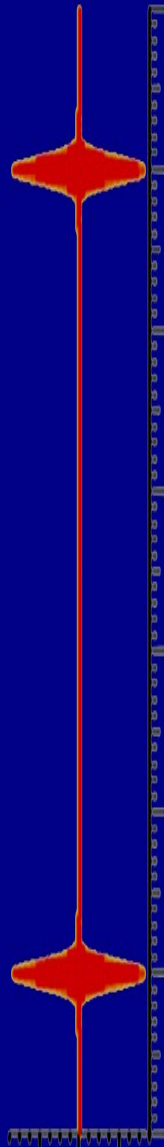

Multiphoton microscopy


Objectives and Detectors

Light must come in to depth
Light must get collected from the depth

Bring back home the photons

Laser → Objective → Excitation

Emission → Objective → Detector

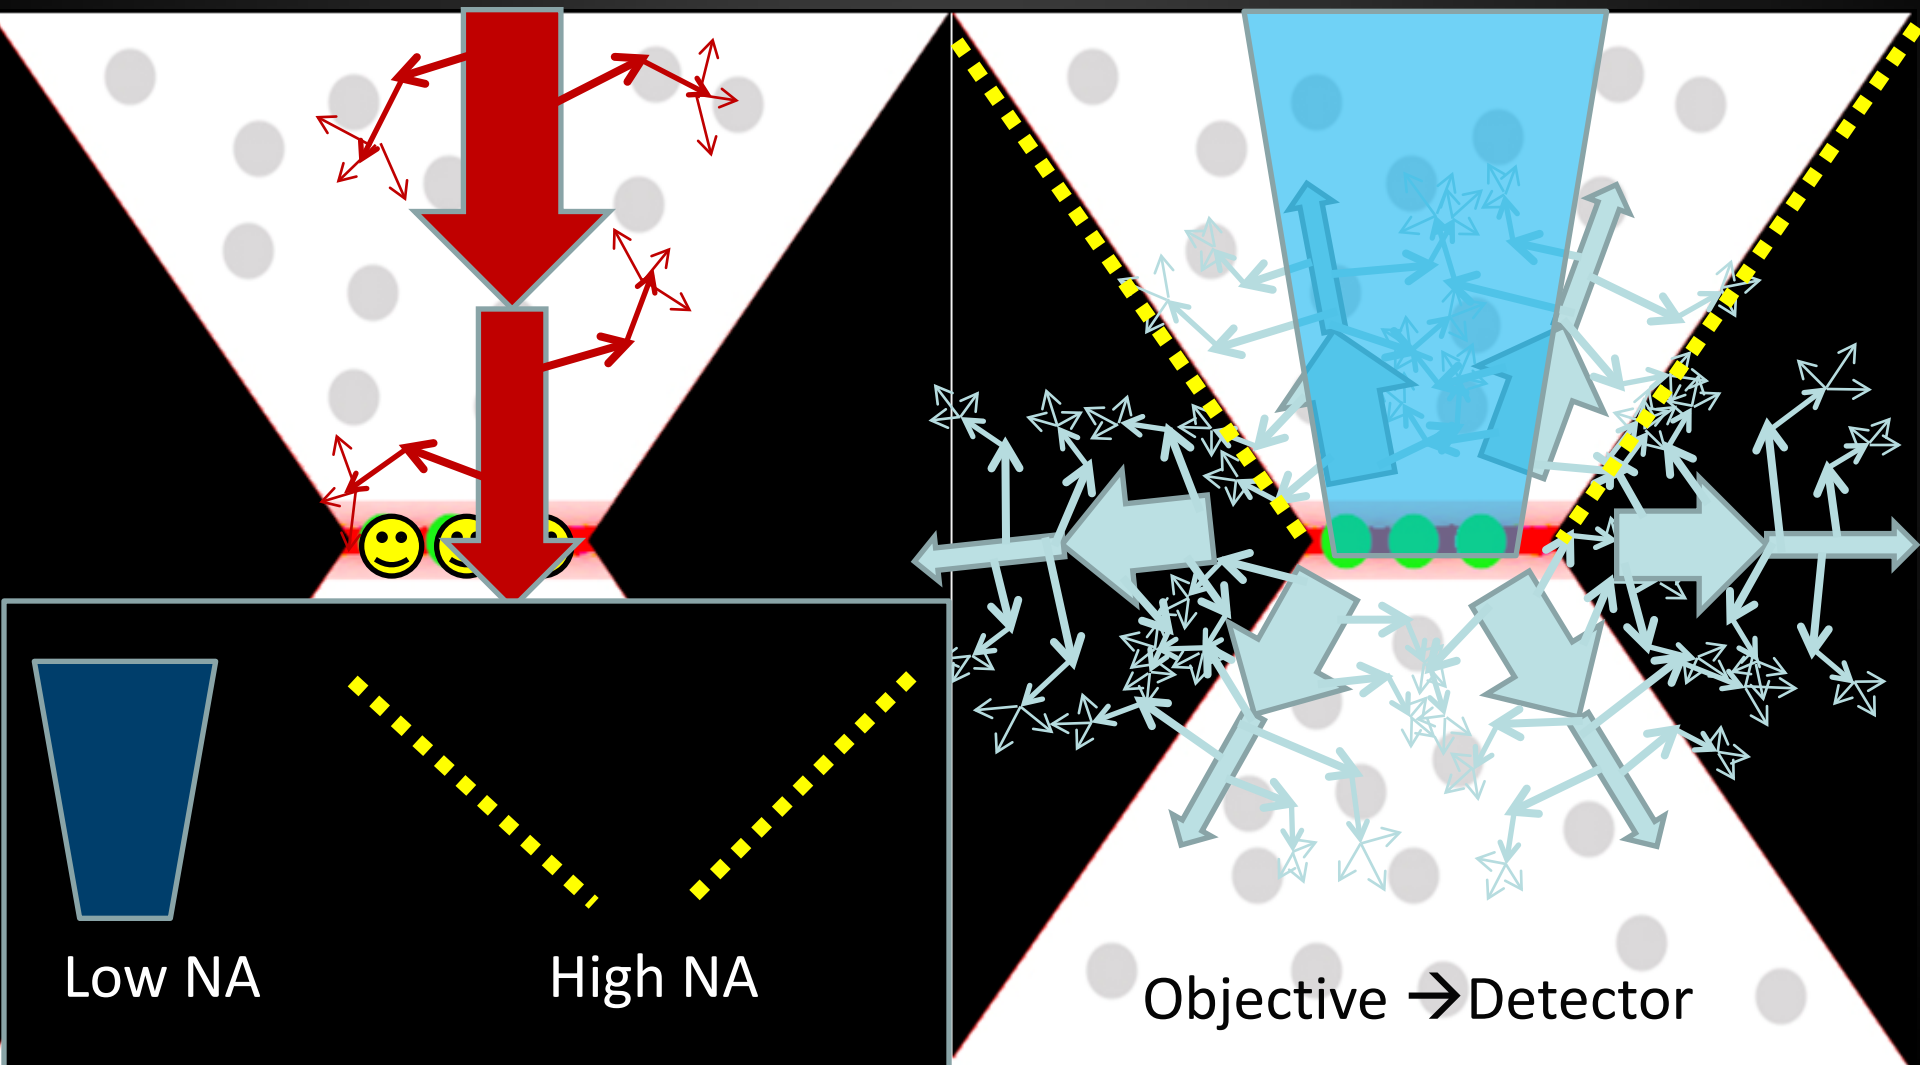

Multiphoton objectives

Long Working distance (2mm) including (!)

High Numerical Aperture

(good resolution/focus, narrow depth of focus)




The Olympus
XLPlan N
25x, NA 1.05



➤ all photons to the focus for high chance of 2P-Ex

- High transmittance and correction for broad range of e.g. 400 nm to 1000 nm
- Water dipping (remember *in vivo* imaging) / cover slip
- Correction collar (!) to compensate for different refractive indices (water 1.3, specimen 1.34-1.4)
- 34 degree angle at lense top for better accessibility to specimen for manipulation

Multiphoton objectives

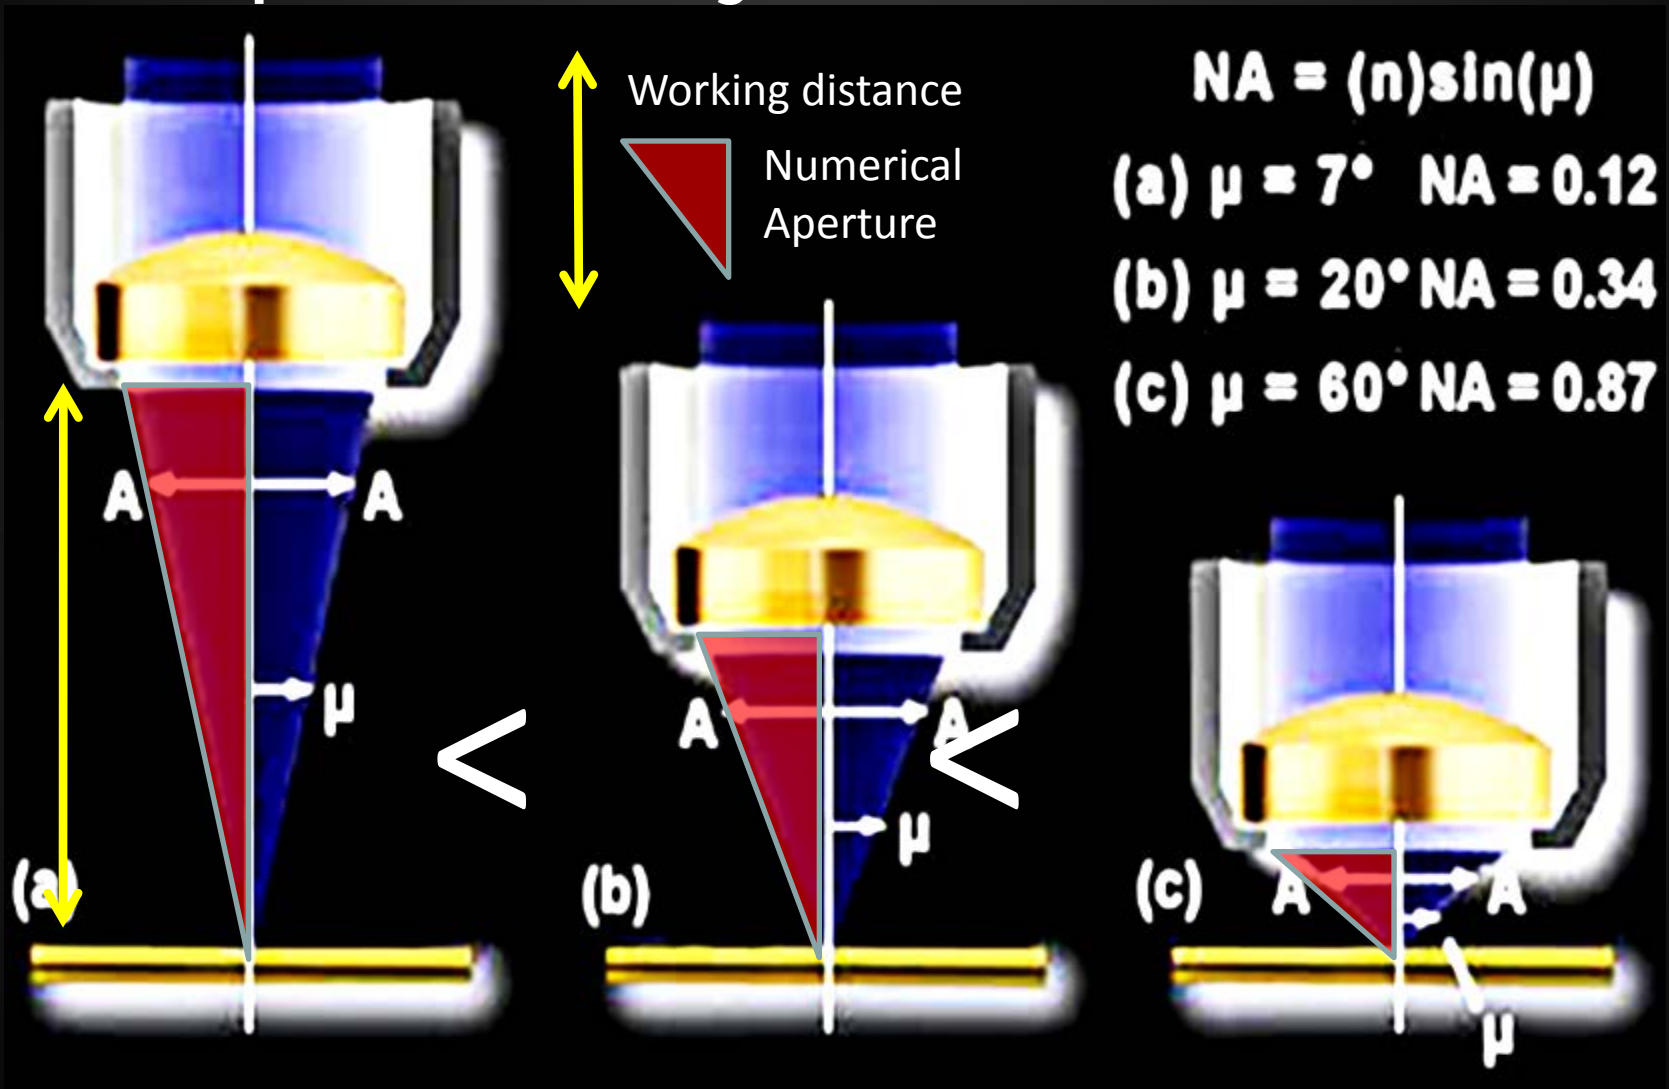

High NA + Long WD = expensive objective

Multiphoton detectors - NDD




Using the "long way" gives more flexibility, the confocal filterfree scanhead can be finetuned what range of light shall be collected, but the way is long (equals 32 cm glas!) and hence **light is lost**...

Using the NDDs as "short cuts" avoids loss of light. NDDs filter light via "old days" filtercubes and therefore lack in flexibility.


Multiphoton detectors - NDD

Loss of emission light: NDD vs LSMD I

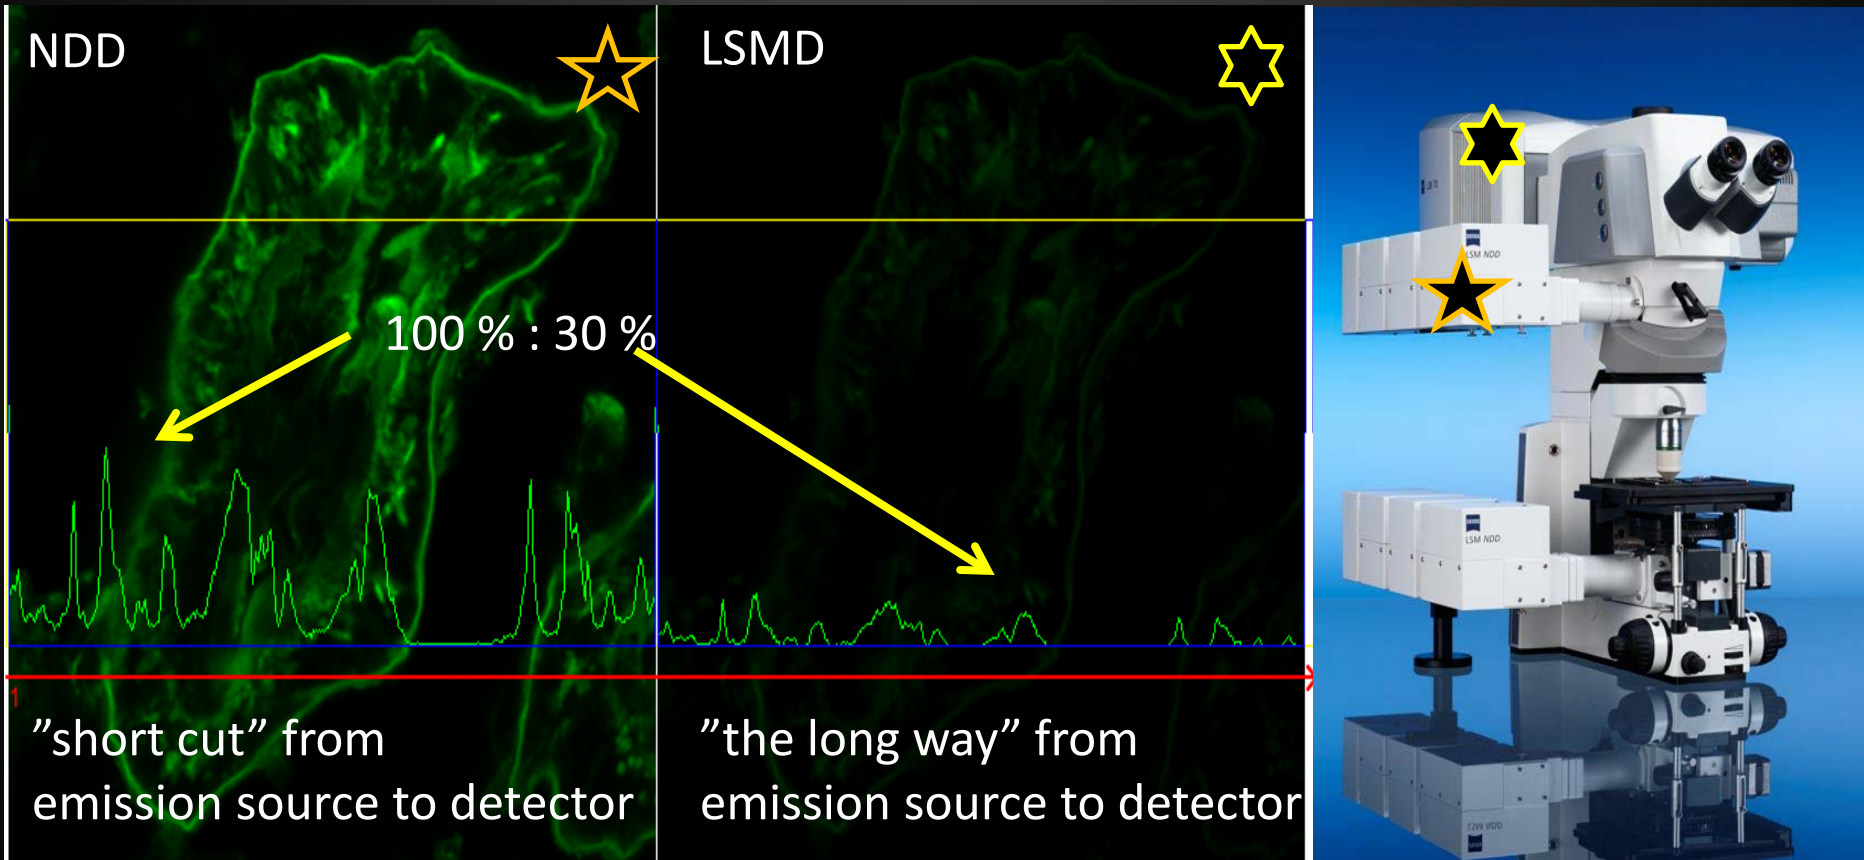

Alexa 488, MaiTai 780nm, 5% (quite high), spectral range emission 500-550nm, no/open pinhole, digital gain etc for NDD (no over/under exposure)


Multiphoton detectors - GaAsP

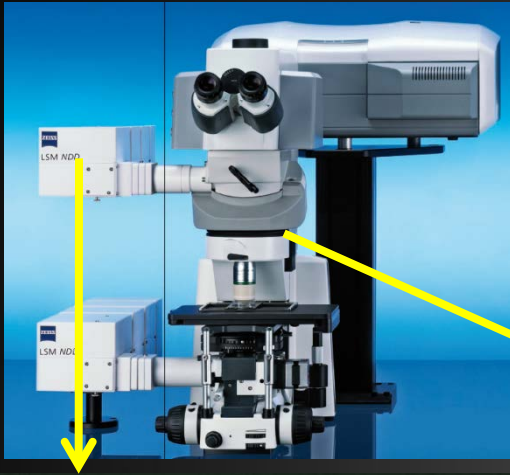


With the very sensitive GaAsP detector right behind the objective we are able to collect more light from weakly fluorescent specimen (higher signal to noise ratio)

- one detector with no filter
- no distinction between different fluorophores...
- Efficiency 40 % for 400 -700 nm

NDD

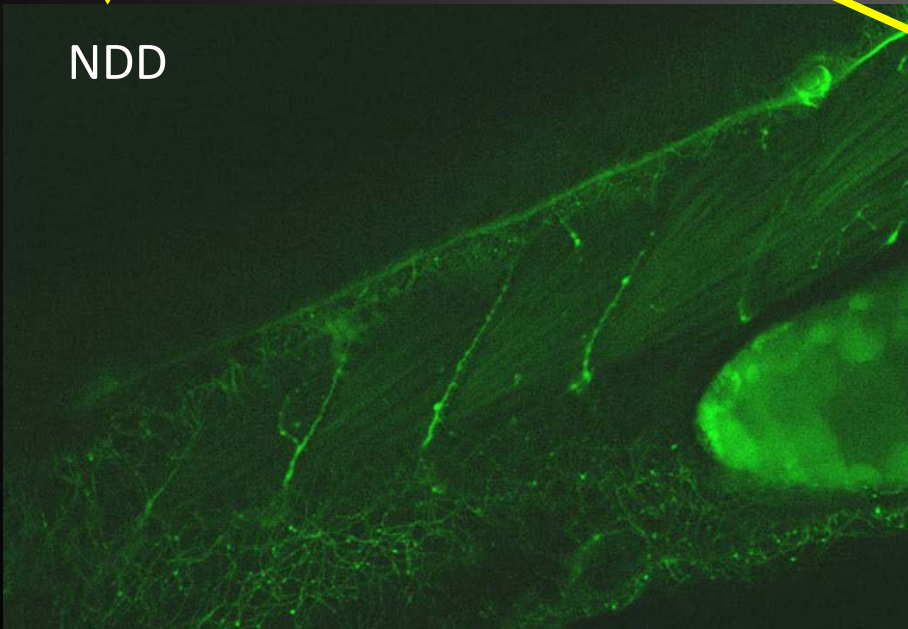

GaASP NDD

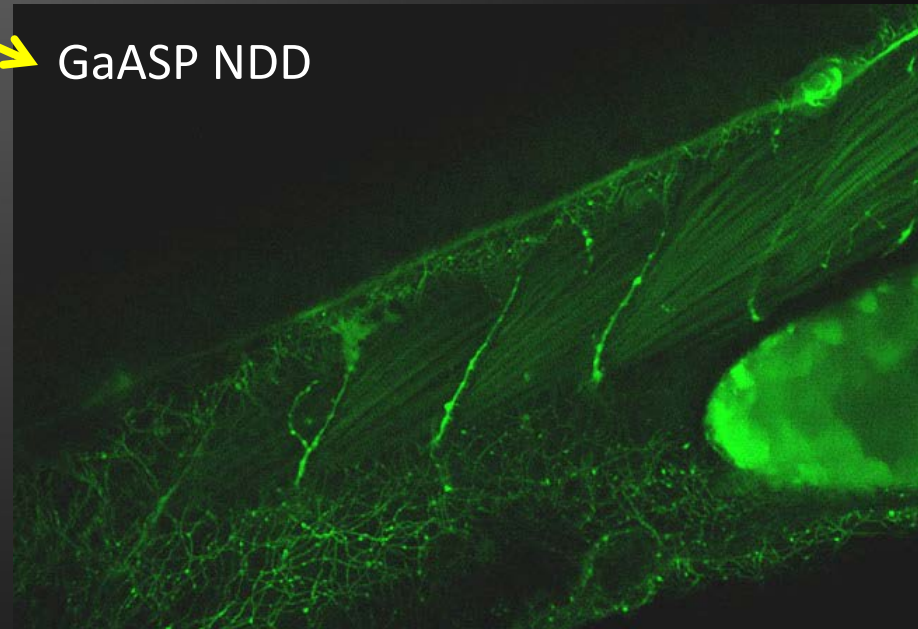

Loss of emission light: NDD vs GaAsP

Bring back home the photons - summary

FL emission is shorter in λ and get more scattered and dispersed than NIR Ex light

➤ Loss of emission light i.e. signal light


light gets lost via the optical pathways

➤ Loss of emission light i.e. signal light

To compensate this loss

Detectors should have

- better sensitivity
- proximity to specimen
- more

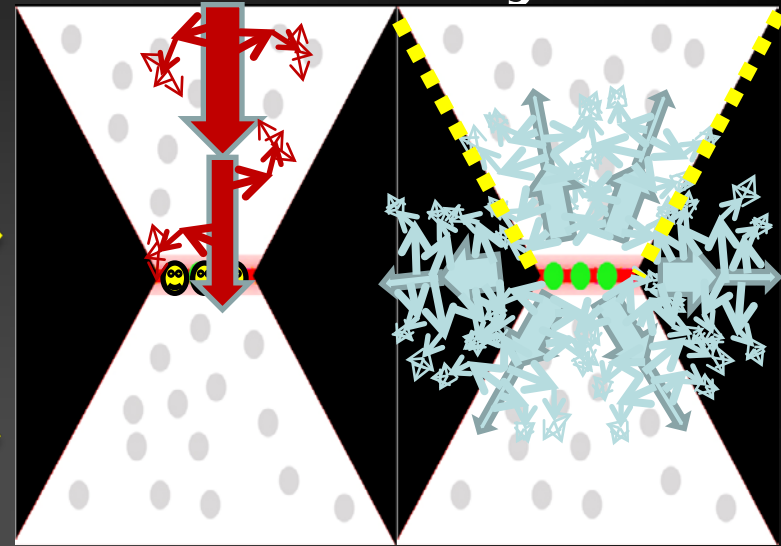

Keep in mind...

A multiphoton microscope gives you the opportunity to get images from **deep** (e.g. 500 nm) within (**living**) tissue, whilst **photodamaging only the imaged volume**.

A Multiphoton microscope is a point scanning system which **excites fluorophores within the Focus volume only**.


Therefore you collect emission light from this volume only, enabling you to acquire optical slices, **without the use of confocal pinholes**.

Beside this, one is able to photomanipulate tissue/cells within a very small volume.

Comparison of CLSM and 2P

	LSM	Multiphoton
light source	laser UV to VIS	tuneable 50-100fs pulsed IR laser
depth of visualization	up to 100 μm depending on tissue	up to 1000 μm depending on tissue
XYZ resolution	via focal plane of objective, pinhole and wavelength	Similar (or worse) as LSM, No pinhole needed
volume of excitation	throughout the illuminated tissue	only the focal plane
sensibility	Loss of signals via optics > Descanned detectors	Enhance signal by use of > Non-descanned detectors

Go deeeeeeeper....

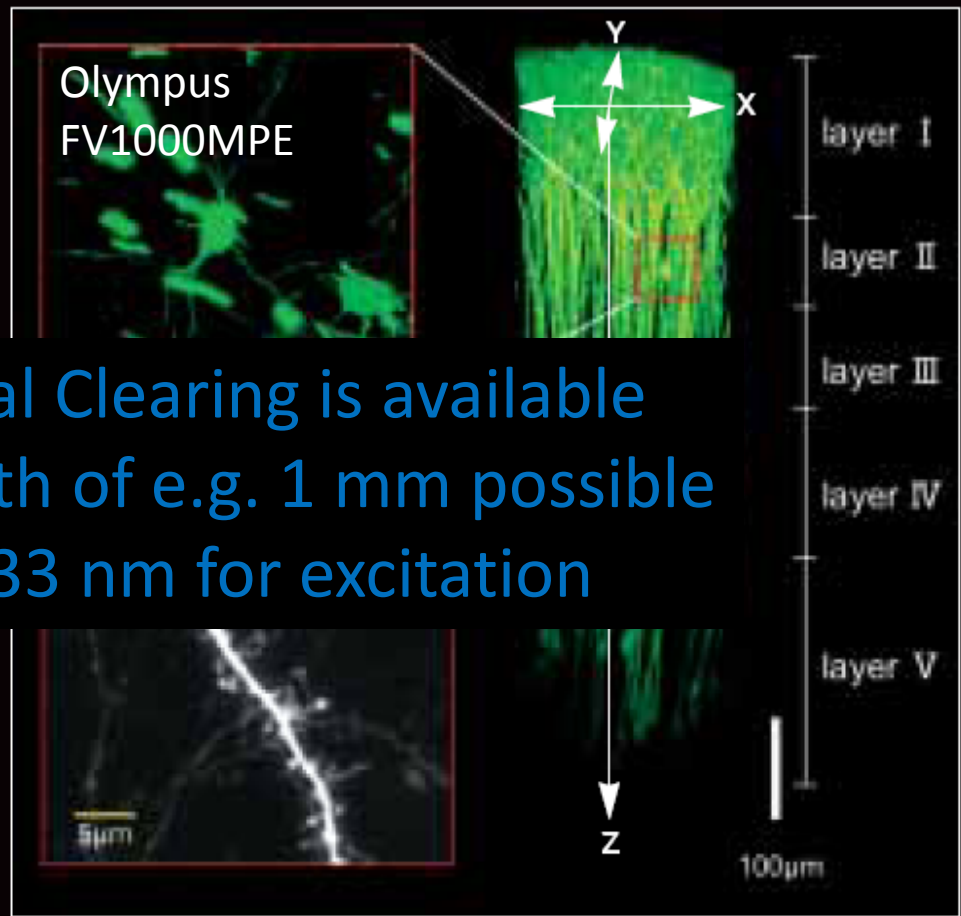

A method called Optical Clearing is available
Making visualization depth of e.g. 1 mm possible
Using light of 300 – 633 nm for excitation



Dendrites of cortical projection neurons of a transgenic mouse expressing YFP via the thyl1 promotor. This high-resolution image of the dendritic processes to a depth of of 430 μm was made using multiphoton excitation of 920 nm in the living animal. Specimen provided by Stephen Turney, MCB, Harvard University, USA



3-dimensionally constructed images of neurons expressing EYFP in the cerebral neocortex of a mouse under anesthesia. Cross-sectional images down to 0.7 mm from the surface can be observed after attachment of a special adapter to the specimen. Objective: LUMPlanFL 60xW/IR
Hiroaki Waki, Tomomi Nemoto, and Junichi Nabekura
National Institute for Physiological Sciences,
National Institutes of Natural Sciences, Japan

app. 600 μm

Optical clearing




Removing the optical barriers (different RIs) makes the object invisible – transparent

- Left: water ($n=1.3$) and glass rod ($n=1.5$)
- Right: oil ($n=1.5$) and glass rod ($n=1.5$)

Optical clearing

ClearT: a detergent- and solvent-free clearing method for neuronal and non-neuronal tissue; <http://dev.biologists.org/content/140/6/1364/F1.expansion.html>

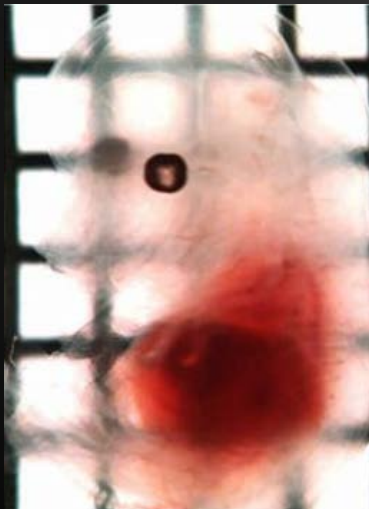

Problem:

Biological tissue : poor light transmission due to interface lipid:water (PM :in/ex-cellular fluids)

Solution:


Replace aqueous fluids with solvents which matches Refractive Index (RI) of lipids.

- Penetration of light into the tissue increases,
- Scattering of light decreases.

Optical Clearing Agents (OCAs) : aromatic hydrocarbons

- water insoluble but soluble in EtOH or MetOH.
- each clearing is preceded by dehydration (Et/MetOH)
- benzyl-alcohol-benzoate (BABB) (excellent)
- Methyl salicylate (wintergreen oil) (very good)
- Thiodiethanol (TDE) (good)
- Glycerin (poor clearing)
- OCAs have usually a refractive index of around 1.5, hence matching RI of glass, and immersion oil.

Optical clearing – go deeper

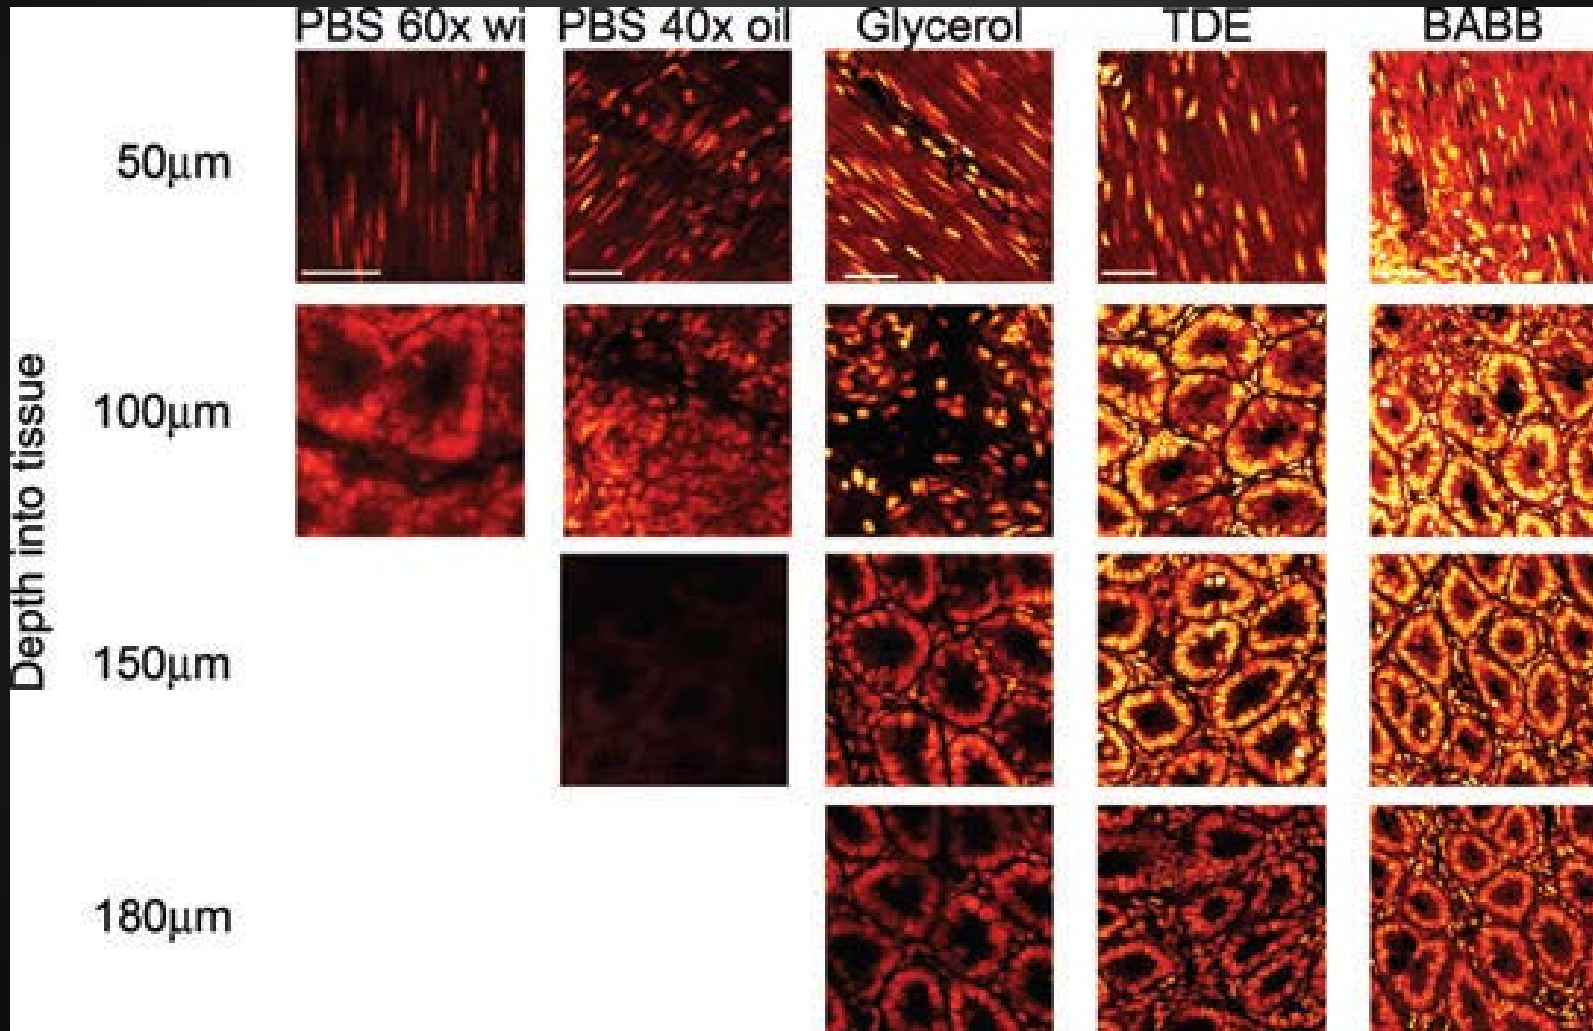

THANKS FOR YOUR ATTENTION!



Ant head autofluorescence

© BioVis – Matyas Molnar